


PHCbi

Operating Instructions

Cooled Incubator

MIR-554 Series

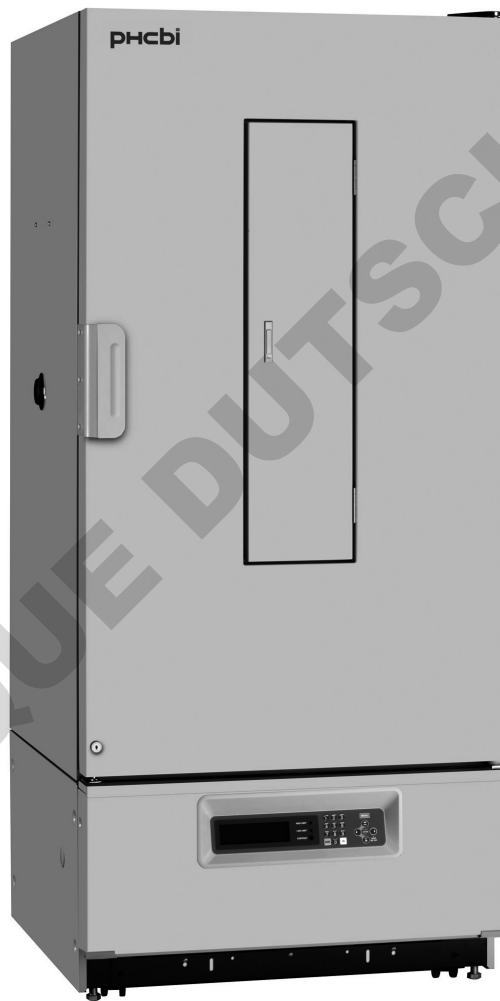

Please read the operating instructions carefully before using this product and keep the operating instructions for future use.

See page 60 for model number.

DOMINIQUE DUTSCHER SAS

CONTENTS

INTRODUCTION	3
PRECAUTIONS FOR SAFE OPERATION	4
SAFE ENVIRONMENTAL CONDITIONS	9
INCUBATOR COMPONENTS	10
Control panel.....	12
Switch box.....	13
INSTALLATION SITE	14
INSTALLATION	15
TOP SCREEN	16
FUNCTIONS THROUGH CONTROL PANEL	17
STANDBY OPERATION (MENU/Std-by)	17
SETTING OF KEY LOCK (MENU/Std-by).....	18
Setting of key lock (Key Lock).....	18
Setting of key unlock (Key Unlock)	18
PROCEDURES OF SETTING VALUE.....	19
Setting of chamber temperature.....	19
Setting of key lock	20
HIGH LIMIT/LOW LIMIT ALARM (MENU/Std-by)	21
PROGRAMMING (MENU/Edit)	22
EDIT OF SAVED PROGRAM (MENU/Edit)	28
START OF PROGRAM (MENU/Run).....	29
JOIN FUNCTION	31
SKIP OF STEP (MENU/Skip).....	32
STOP OF PROGRAM (MENU/Stop).....	33
AUTOMATIC DEFROST (MENU/Tools/Date Time).....	34
MANUAL DEFROST (MENU/M.def)	35
VARIOUS SETTING (MENU/Tools).....	36
Display of log (Tools/Log)	36
Setting of date, time, log (Tools/Date Time).....	39
Alarm setting (Tools/Alarm, Opt., Low Humi. Setting)	40
Key lock password setting (Tools/Key Lock PW Setting)	41
Default setting (Tools/Default Setting)	42
Delete of program (Tools/Delete User Data).....	43
ADJUSTMENT OF SHELVES.....	45
ALARMS AND SAFETY FUNCTIONS	46
MAINTENANCE	49
Cleaning.....	49
Cleaning of evaporating tray.....	50

CONTENTS

TROUBLESHOOTING	51
DISPOSAL OF UNIT	52
Refrigerant (applicable to MIR-554-PE).....	52
LOW HUMIDITY MODE	57
PERFORMANCE DATA.....	58
SPECIFICATIONS.....	59
PERFORMANCE.....	60
SAFETY CHECK SHEET	61

DOMINIQUE DUTSCHER SAS

INTRODUCTION

- Read the operating instructions carefully before using the Product and follow the instructions for safety operation.
- PHC Corporation disavows any responsibility for safety if the Product is used for other than the intended use or used with any procedures other than those given in the operating instructions.
- Keep the operating instructions in a suitable place so that it can be referred to as necessary.
- The contents of the operating instructions are subject to change without notice for improvement of performance or functions.
- Contact our sales representative or agent if any page of the operating instructions is lost or the page order is incorrect.
- Contact our sales representative or agent if any point in the operating instructions is unclear or if there are any inaccuracies.
- No part of the operating instructions may be reproduced in any form without the expressed written permission of PHC Corporation.

IMPORTANT NOTICE

PHC Corporation guarantees this product under certain warranty conditions. However, please note that PHC Corporation shall not be responsible for any loss or damage to the contents of the product.

<Intended Use>

This product is laboratory equipment intended to carry out bacteria test, food abuse test, constant-temperature test, and culture of microorganism, etc.

PRECAUTIONS FOR SAFE OPERATION

It is imperative that the user comply with the operating instructions as they contain important safety advice.

Items and procedures are described so that you can use this unit correctly and safely. If the precautions advised are followed, this will prevent possible injury to the user and any other person.

Precautions are illustrated in the following way:




WARNING

Failure to observe WARNING signs could result in a hazard to personnel possibly resulting in serious injury or death.

CAUTION

Failure to observe CAUTION signs could result in injury to personnel and damage to the unit and associated property.

Symbol shows;






-  This symbol means caution.
-  This symbol means an action is prohibited.
-  This symbol means an instruction must be followed.

For the State of California, USA Only:

This product contains a CR Coin Cell Lithium Battery which contains Perchlorate Material – special handling may apply. See www.dtsc.ca.gov/hazardouswaste/perchlorate.















SYMBOLS ON UNIT

The following symbols are attached to the unit. The table describes the meaning of the symbols.

	This symbol is attached to covers that access high-voltage electrical components to prevent electric shock. Only a qualified engineer or service personnel should be allowed to open these covers.
	This symbol indicates that caution is required. Refer to product documentation for details.
	This symbol indicates a hot surface.
	This symbol indicates an earth.
	This symbol indicates incorrect usage could lead to a fire hazard.
	This symbol means "ON" for a power switch.
○	This symbol means "OFF" for a power switch.

PRECAUTIONS FOR SAFE OPERATION

WARNING


-  **Do not use the unit outdoors.** Current leakage or electric shock may result if the unit is exposed to rain water.
-  **Only qualified engineers or service personnel should install the unit.** The installation by unqualified personnel may cause electric shock or fire.
-  **Install the unit on a sturdy floor and take an adequate precaution to prevent the unit from turning over.** If the floor is not strong enough or the installation site is not adequate, this may result in injury from the unit falling or tipping over.
-  **Never install the unit in a humid place or a place where it is likely to be splashed by water.** Deterioration of the insulation may result which could cause current leakage or electric shock.
-  **Never install the unit in a flammable or volatile location.** This may cause explosion or fire.
-  **Never install the unit where acid or corrosive gases are present** as current leakage or electric shock may result due to corrosion.
-  **Always ground (earth) the unit to prevent electric shock.** If the power supply outlet is not grounded, it will be necessary to install a ground by qualified engineers.
-  **Never ground the unit through a gas pipe, water main, telephone line or lightning rod.** Such grounding may cause electric shock in the case of an incomplete circuit.
-  **Connect the unit to a power source as indicated on the rating label attached to the unit.** Use of any other voltage or frequency other than that on the rating label may cause fire or electric shock.
-  **Never store volatile or flammable substances** in this unit if the container cannot be sealed. These may cause explosion or fire.
-  **Do not insert metal objects such as a pin or a wire into any vent, gap or any outlet on the unit.** This may cause electric shock or injury by accidental contact with moving parts.
-  **Use this unit in safe area when treating the poison, harmful or radiate articles.** Improper use may cause bad effect on your health or environment.
-  **Turn off the power switch (if provided) and disconnect the power supply to the unit prior to any repair or maintenance** of the unit in order to prevent electric shock or injury.
-  **Do not touch any electrical parts (such as power supply plug) or operate switches with a wet hand.** This may cause electric shock.

WARNING

-  **Ensure you do not inhale or consume medication or aerosols** from around the unit at the time of maintenance. These may be harmful to your health.
-  **Never splash water directly onto the unit** as this may cause electric shock or short circuit.
-  **Never put containers with liquid on the unit** as this may cause electric shock or short circuit when the liquid is spilled.
-  **Never bind, process, or step on the power supply cord, or never damage or break the power supply plug.** A broken power supply cord or plug may cause fire or electric shock.
-  **Do not use the power supply cord if its power supply plug is loose.** Such power supply cord may cause fire or electric shock.
-  **Never disassemble, repair, or modify the unit yourself.** Any such work carried out by an unauthorized person may result in fire, or electric shock or injury due to a malfunction.
-  **Disconnect the power supply plug if there is something wrong with the unit.** Continued abnormal operation may cause electric shock or fire.
-  **When removing the power supply plug from the power supply outlet, grip the power supply plug, not the cord.** Pulling the power supply cord may result in electric shock or fire by short circuit.
-  **Disconnect the power supply plug** before moving the unit. Take care not to damage the power supply cord. A damaged power supply cord may cause electric shock or fire.
-  **Disconnect the power supply plug when the unit is not used for long periods.** Keeping the connection may cause electric shock, current leakage, or fire due to the deterioration of insulation.
-  **If the unit is to be stored unused in an unsupervised area for an extended period, ensure that children do not have access and that doors cannot be closed completely.**
-  **Ask a qualified contractor to carry out disassembly and disposal of the unit.** Leaving the unit in a location that can be accessed by third parties may result in unexpected accidents (e.g. the unit may be used for unintended purposes).
-  **Do not put the packing plastic bag within reach of children** as suffocation may result.
-  **Do not position this unit and the other unit so that it is difficult to operate the disconnection of the power supply plug.** Failure to disconnect the power supply plug may cause fire if there is something wrong with the unit.

PRECAUTIONS FOR SAFE OPERATION

WARNING


 **Install the unit in a well-ventilated (airy) location to prevent the accumulation of flammable refrigerant.** The flammable refrigerant may cause fire if it leaks.

Flammable and explosive product



The unit contains flammable refrigerant. When repairing or recycling, only trained service personnel will repair and follow the procedure below.

- Well ventilate the room to prevent refrigerant accumulation.
- Keep fire away when the refrigerant is contained in the product.
- Do not damage or break the pipework.
- When replacing parts, use parts of the same type.
- The appliance shall be stored in a room without continuously operating ignition sources (for example: open flames, an operating gas appliance or an operating electric heater).
- Do not pierce or burn.
- Be aware that refrigerants may not contain an odour.


 **The unit contains flammable refrigerant and flammable blowing gas. When the unit is disassembled or disposed of, the work must be performed in a well-ventilated place and avoid the place near fire.**
It may cause explosions and/or a fire in case of refrigerant or gas leakage.


 **Do not give strong shock or vibration during movement or use.** The piping may be damaged, causing a fire.


 **Do not use electrical appliances in the chamber.** If the refrigerant leaks, sparks from the electrical contacts could cause a fire or explosion.


CAUTION


 This unit must be plugged into a dedicated circuit protected by branch circuit breaker.

 Use a dedicated power source as indicated on the rating label attached to the unit. A multiple-tap may cause fire resulting from abnormal heating.

 **Never store corrosive substances such as acid or alkali** in this unit if the container cannot be sealed. These may cause corrosion of inner components or electric parts.

 **Check the setting when starting up of operation after power failure or turning off of power switch.** The stored items may be damaged due to the change of setting.


 **Be careful not to tip over the unit** during movement to prevent damage or injury.

 **Prepare a safety check sheet** (copy the last page) when you request any repair or maintenance for the safety of service personnel.

Flammable and explosive product



The unit contains flammable refrigerant. Consult repair manual/owner's guide before attempting to install or service this product. All safety precautions must be followed.

 **Flammable refrigerant is used.** Dispose of the unit properly in accordance with national or local regulations.

SAFE ENVIRONMENTAL CONDITIONS

This equipment is designed to be safe at least under the following conditions:

- Indoor use;
- Altitude up to 2000 m;
- Temperature 5 °C to 40 °C;
- Maximum relative humidity 80 % for temperature up to 31 °C decreasing linearly to 50 % relative humidity at 40 °C;
- Mains supply voltage fluctuations up to ± 10 % of the nominal voltage;
- Transient overvoltages up to the levels of OVERVOLTAGE CATEGORY II;
- Temporary OVERVOLTAGES occurring on the mains supply;
- Applicable pollution degree of the intended environment (POLLUTION DEGREE 2 in most cases);

* The above conditions do not indicate the performance of this product. For the performance of this product, refer to the "PERFORMANCE" section.

INCUBATOR COMPONENTS



1. Shade: To protect the lamp.

2. Door: The door can be opened to 130 degrees approx. The door is sealed securely to the cabinet by the magnetic gasket when it is closed.

Condensation may occur at the inner side of the door when a lot of damp material stored.

3. Door switch: To prevent the air from escaping by stopping the air circulating fan when the door is opened.

4. Glass window: 3-layer heat-absorbing glass to shut out the heat.

5. Shelf: The location (height) is adjustable according to the item size to be stored.

Do not change the position of the lowest shelf or do not remove the stainless panel on the lowest shelf to keep original airflow inside the chamber.

6. Keyhole: Insert the key and turn 180 degrees to the left, and the door is locked.

7. Leveling foot: Use these bolts to adjust the height and level the unit for installation.

8. Evaporating tray: The drained water resulting from the defrosting is accumulated and evaporated automatically in this tray. (Page 50)

9. Frost check opening: Check the frost on the condenser through this opening.

10. Access port: This port allows cables to be passed into the cabinet.

Note: Be sure to set the rubber stopping to the access port (placed at the left and right side) as it was when passing cables for measurement and power cords through it.

Be sure to replace the cap after take out cable or, the inside temperature cannot complete down, and frost may accumulate outside the port surroundings.

11. Air blowing duct: The heat-exchanged air is blown out from this duct.

12. Air circulating fan: Fan is installed inside the duct. Do not insert anything into the duct.

13. Drain port: Use this port when the chamber is washed with water. Always cover the port with cap when no use.

14. Switch box: Power switch, and remote alarm terminals placed.

15. Control panel: Temperature control, alarm setting, program setting are available through the control panel. The temperature indicator is attached on the control panel.

16. Glass protective plate: This prevents glass cracking.


17. Dew saucer: To hold the dew that adhere to inside of the door.

18. Caster: To facilitate the moving of the cabinet.

19. Port for drain pipe: To take out the drain pipe to avoid the overflow of the evaporating tray in the case of long term humidity operation. (Page 57)

INCUBATOR COMPONENTS

Control panel

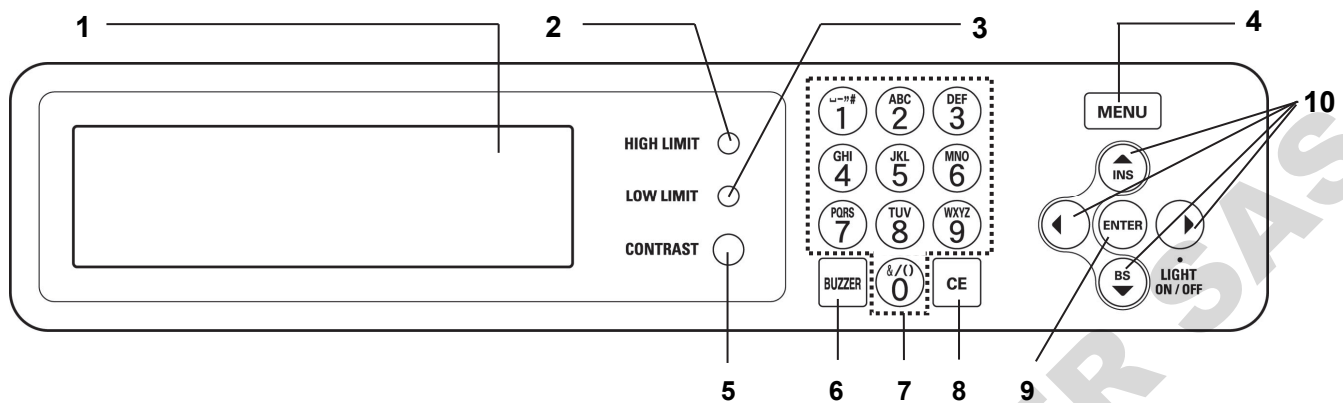

1. LCD panel

2. High limit temperature alarm volume (HIGH LIMIT)

To set the temperature of high limit temperature alarm.

3. Low limit temperature alarm volume (LOW LIMIT)

To set the temperature of low limit temperature alarm.

4. Menu button (MENU)

To open the menu window.

5. LCD contrast adjusting knob (CONTRAST)

To adjust the contrast of LCD.

6. Alarm buzzer stop key (BUZZER)

To silence the alarm buzzer temporarily.

7. Character input key

8. Clear key (CE)

To clear the input value during editing of program.

9. Enter key (ENTER)

To determine the selection of menu. In program editing, pressing this key causes moving to the next article.

10. Shift key (Upward, downward, rightward, leftward)

Upward: To move the cursor upward. (When inputting a program name: Space key)


Downward: To move the cursor downward. (When inputting a program name: BackSpace key)

Leftward: To move the cursor leftward.

Rightward: To move the cursor rightward. (When displaying the top screen: lamp ON/OFF*.)

*The lighting is available only with temperature range between +2 °C and +50 °C when the optional Light add on kit (MIR-L15) is installed.

Switch box

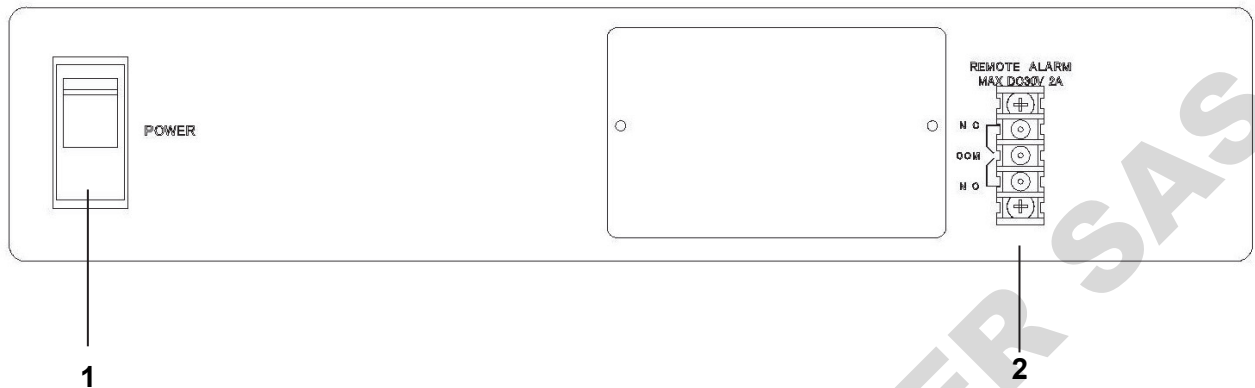

1. Power switch (POWER)

The switch for ON/OFF of all power source.

2. Remote alarm terminals

Alarm signal can be drawn out via the contact output. Permissible contact capacity: DC 30 V, 2 A

- a) Contact output: Connect the lead wires to COM and NO terminals.
(Normal condition: open. Abnormal condition: close.)
- b) Contact output: Connect the lead wires to COM and NC terminals.
(Normal condition: close. Abnormal condition: open.)

COM and NO terminals are closed at the failure of electricity supply.

Note:

- It is recommended to use standard signal and interface cables with a maximum length of 30 meters.

INSTALLATION SITE

To operate this unit properly and to obtain maximum performance, install the unit in a location with the following conditions:

■ **A location not subjected to direct sunlight**

Do not install the unit under direct sunlight. Installation in a location subjected to direct sunlight cannot obtain the intended performance.

■ **A location with adequate ventilation**

Leave at least 10 cm around the unit for ventilation. Poor ventilation will result in a reduction of performance and consequently failure.

■ **A location away from heat generating sources**

Avoid installing the unit near heat-emitting appliances such as a heater or a boiler etc. Heat can decrease the intended performance of the unit.

■ **A location with little temperature change**

Install the unit under stable ambient temperature. The allowable ambient temperature is between +5 °C and +35 °C.

Note: This incubator changes to PID control when the temperature setting is about 10 °C higher than the ambient temperature. Under PID control, the temperature cycle is very small. For other temperature setting, the incubator is operated with ON-OFF control, which temperature cycle is about 3 °C. At the beginning of operation or when the ambient temperature is fairly high, the cabinet side may heat up. However, this does not denote a malfunction. It is due to the hot gas piped around the unit frame to prevent condensation around the cabinet.

■ **A location with a sturdy and level floor**

Always install the unit on a sturdy and level floor. The uneven floor or tilted installation may cause failure or injury. Install the unit in stable condition to avoid vibration or noise. Unstable condition may cause vibration or noise.

 **WARNING**

Install the unit on a sturdy floor. If the floor is not strong enough or the installation site is not adequate, this may result in injury from the unit falling or tipping over.

Select a level and sturdy floor for installation. This precaution will prevent the unit from tipping. Improper installation may result in water spillage or injury from the unit tipping over.

■ **A location not prone to high humidity**

Install the unit in the ambient of 80 %R.H. or less humidity. Installation under high humidity may cause current leakage or electric shock.

 **WARNING**

Do not use the unit outdoors. Current leakage or electric shock may result if the unit is exposed to rain water.

Never install the unit in a humid place or a place where it is likely to be splashed by water. Deterioration of the insulation may result which could cause current leakage or electric shock.

■ **A location without flammable or corrosive gas**

Never install the unit in a flammable or corrosive location. This may cause explosion or fire or may result in the current leakage or electric shock by the corrosion of the electrical components.

⚠ CAUTION

Do not install it on the place (near the drain facilities etc.) where the corrosion cause material like the sulfur compound etc. might be generated. The refrigeration unit is deteriorated, and it causes the breakdown of the product due to the corrosion of the copper pipe.

■ A location where nothing falls on

Do not install the product where things might fall on it. The product might be damaged, and it causes a breakdown.

INSTALLATION

1. Remove the door fixture

Loosen 4 screws and remove the door fixture at the top left of the cabinet.

2. Remove the packaging materials and tapes

Remove all transportation packaging materials and tapes. Open the doors and ventilate the unit. If the outside panels are dirty, clean them with a diluted neutral dishwashing detergent. (Undiluted detergent can damage the plastic components. For the dilution, refer to the instruction of the detergent.) After cleaning with the diluted detergent, always wipe it off with a wet cloth. Then wipe off the panels with a dry cloth.

Note:

Remove the cable tie banding the power supply cord. Prolonged banding may cause the corrosion of the cord coating.

3. Adjust the leveling foot

Extend the leveling feet by rotating them counterclockwise to contact them to the floor. Ensure the unit is level.

4. Ground (earth)


⚠ WARNING

Use a power supply outlet with ground (earth) to prevent electric shock. If the power supply outlet is not grounded, it is necessary to install a ground by qualified engineers.

Never ground the unit through a gas pipe, water main, telephone line or lightning rod. Such grounding may cause electric shock in the case of an incomplete circuit.


Note:

The chamber temperature may deviate from the set temperature when the unit is running with the heater or motor energized.

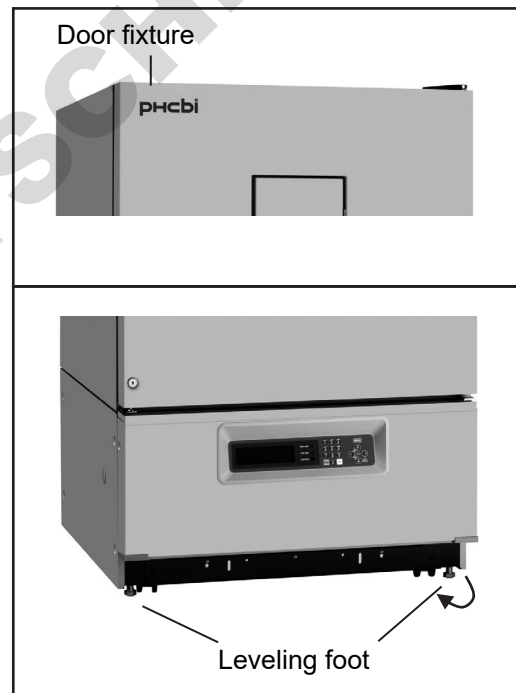

TOP SCREEN

The top screen below is displayed when turning on the power switch. The default temp. is 25.0 °C. The date and time are preset at the factory. Refer to page 39 when more accurate setting is needed.

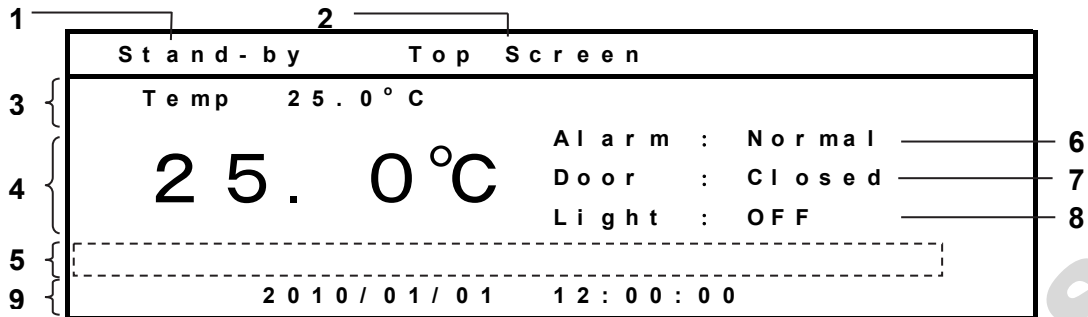

1. Display of running status

The current running status is displayed. At the power-on, "stand-by" is displayed and the system runs continuously under the stand-by running condition (refer to page 17). When turning on power for the first time, the system runs continuously under the initial setting condition.

"Running" is displayed at the time of programmed running. "Defrosting" is displayed with reversed and non-reversed character alternately while removing frost.

"Low Humi." is displayed with reversed and non-reversed character alternately while low humidity mode.

2. Display of program name

A program name under operation is displayed. "Top Screen" is displayed during standby operation.

3. Display of setting

Set value of temperature is displayed.

4. Display of current value

Current value of temperature is displayed.

5. Message display field

A message is displayed when a breakdown occurs.

6. Alarm display (Alarm)

"Alarm" is alternately displayed by reversed/non-reversed character while alarm is operating.

"Warning" is alternately displayed by reversed/non-reversed character at the time of warning.

"Normal" is displayed at a normal condition.

An adding message is displayed in the message display field.

7. Display of door status

"Door" is highlighted when the door is open. "Closed" is displayed when the door is closed.

8. Lighting display (Light)

"ON" is displayed in outline type when the lighting has been turned on. "OFF" is displayed when turned off. When the lighting is set to be turned on, the system is programmed running, "Program_ON" is displayed in outline type when the lighting has been turned on and "Program_OFF" is displayed in outline type when the lighting has been turned off.

9. Display of date and time

The current date and time is displayed.

FUNCTIONS THROUGH CONTROL PANEL

The following functions are available through control panel:

- **Setting of standby operation:** To set a running condition at the start-up or completion of programmed running. (refer to page 17)
- **Programming and edit:** To set a new program (page 22), or to edit (page 28), or delete (page 43) a user program.
- **Programmed running:** To start (page 29), skip (page 32) or stop (page 33) a programmed running.
- **Setting of defrost:** To set the automatic defrost (page 34) and to start the manual defrost. (page 35)
- **Setting of log cycle and sending to PC:** To set a log cycle of running data and to send a running log to PC. (page 38)
- **Setting of date and time:** To set the date and time shown on the top screen. (page 39)
- **Setting of alarm:** To set temperature alarm (page 40) and a high limit (or low limit) temperature alarm. (page 21)
- **Setting for optional component:** To set when an optional component is installed. (page 40)
- **Setting of low humidity mode:** To set the running for low humidity. (page 40)
- **Default setting:** To set the default for LCD panel and communication (DAQ) speed etc. (page 42)

STANDBY OPERATION (MENU/Std-by)

This product automatically operates with standby operation setting.

1. With the top screen displayed, press the menu button (MENU) to show the menu window. Select "Std-by" and press the enter key (ENTER).

Stand-by Top Screen		MENU
Temp 25.0°C	Alarm : Nor	Run
25.0°C	Door : Clo	Std-by
	Light : OFF	Edit
		Tools
2010/01/01	12:00:00	M. Def

2. Stand-by Setting screen is displayed. Set each parameter.

Stand-by Setting	
Temperature	25.0°C (-10.0°C - +60.0°C)
Light Step	0LS (0.OFF 1.ON)
Key Lock	0 (0.UnLock 1.Lock)
High Limit	65°C
Low Limit	-15°C

3. Press the menu button (MENU) at the completion of parameter setting. The menu window is shown. Select "OK" and press the enter key (ENTER). The parameter is memorized.

The settable range of each parameter:

- Temperature: -10°C~60°C

*The settable range and screen display is -10°C~+50°C when the optional inner door (MIR-55ID) is installed.

STANDBY OPERATION (MENU/Std-by)

■ Light step: 1 (ON) or 0 (OFF). In the case of selecting 0 (OFF), by pressing the rightward shift key, lighting is turned on or off when the top screen is displayed.

(While the program operates, on/off of lighting depends on the program.)

*The lighting is available only with temperature range between +2°C and +50 °C when the optional light add on kit (MIR-L15) is installed.

■ Key Lock: When selecting 1 (Lock), it is not possible to change any parameter. To unlock, it is required to input the key lock password.

Refer to the next for the details.

SETTING OF KEY LOCK (MENU/Std-by)

Setting of key lock (Key Lock)

1. When setting of key lock, change the value of the key lock line from “0” to “1” in the stand-by setting screen (Stand-by Setting) and press the enter key (ENTER). The buzzer rings for a short while, and then the key is locked.

Stand-by Setting	
Temperature	25.0°C (-10.0°C - +60.0°C)
Light Step	0LS (0.OFF 1.ON)
Key Lock	1 (0.UnLock 1.Lock)
High Limit	65°C
Low Limit	-15°C

2. The other settings except key lock cannot be changed.

Setting of key unlock (Key Unlock)

1. When setting of key unlock, change the value of the key lock line from “1” to “0” in the stand-by setting screen (Stand-by Setting) and press the enter key (ENTER).

Stand-by Setting	Key Lock
Temperature	25.0°C (-10.0°C - +60.0°C)
Light Step	0LS (0.OFF 1.ON)
Key Lock	0 (0.UnLock 1.Lock)
High Limit	65°C
Low Limit	-15°C

2. Input password of 4 digits to the password field (Password) where the cursor is moved to and press the enter key (ENTER). When setting of key unlock, the buzzer rings for a short while, and then “Key Lock” disappears in the stand-by setting screen (Stand-by Setting).

Stand-by Setting	Key Lock
Temperature	25.0°C (-10.0°C - +60.0°C)
Light Step	0LS (0.OFF 1.ON)
Key Lock	0 Password ****
High Limit	65°C
Low Limit	-15°C

Caution:

The buzzer rings for a long time when a wrong password is input. Input a correct password.
 The password for key unlock must be shared and administered by all users on this product.
 The duration is set in "0000" at the factory.
 Refer to page 41 for changing the password.

PROCEDURES OF SETTING VALUE

Setting of chamber temperature

Procedures of changing chamber temperature from 25 °C to -10 °C are shown below. As for other values, the same procedure is applied.

Procedures of changing chamber temperature from 25 °C to -10 °C

	Operation	Key	LCD Display
1		----	Top screen is displayed.
2	Press the menu button (MENU).	MENU	MENU window is displayed.
3	Select Std-by in MENU window pressing the shift key (downward).	▼	Std-by is displayed in white letters.
4	Press the enter key (ENTER).	ENTER	Stand-by Setting screen is displayed and chamber temperature setting value is changed into white letters.
5	Change the value from 25.0 to 10.0 pressing the character input key.	1 0 0	Chamber temperature setting value 10.0 is displayed.
6	Press the menu button (MENU).	MENU	MENU window is displayed.
7	Select +/- in MENU window pressing the shift key (downward).	▼	+/- is displayed in white letters.
8	Press the enter key (ENTER).	ENTER	Chamber temperature setting value -10.0 is displayed.
9	Press the enter key (ENTER).	ENTER	Next item (Light Step) is displayed in white letters.
10	Press the menu button (MENU).	MENU	MENU window is displayed. OK is already selected (displayed in white letters).
11	Press the enter key (ENTER).	ENTER	The set value is memorized, and top screen is displayed.

CAUTION

The settable range of chamber temperature is between -10 °C and +60 °C.

- The lighting is available only with temperature range between +2 °C and +50 °C when the optional light add on kit (MIR-L15) is installed. In the case of temperature out of range, the lighting is not usable. The lamp is off with the temperature out of range when the saved program is running.

In this case, temperature fluctuation may exceed ±1.5 °C or it may take longer time to pull down the chamber temperature.

- The temperature control range is -10 °C~+50 °C when the optional inner door (MIR-55ID) is installed. The temperature is limited to 50 °C when the saved program includes temperature setting over 50 °C. In this case, the temperature setting over 50 °C is indicated by blinking.

PROCEDURES OF SETTING VALUE

Setting of key lock

Procedures of changing Key Lock setting are shown below.

Procedures of Key Lock (Changing Key Lock setting from 0(Unlock) to 1(Lock)).

	Operation	Key	LCD Display
1		----	Top screen is displayed.
2	Press the menu button (MENU).	MENU	MENU window is displayed.
3	Select Std-by in MENU window pressing the shift key (downward).	▼	Std-by is displayed in white letters.
4	Press the enter key (ENTER).	ENTER	Stand-by Setting screen is displayed and chamber temperature setting value is changed into white letters.
5	Select Key Lock item pressing Shift keys.	▼	Set value of (Key Lock) is displayed in white letters.
6	Change the value from 0 to 1 pressing the character input key.	1	Set value "1" is displayed.
7	Press the enter key (ENTER).	ENTER	The value of top item (Temperature) is displayed in white letters. "Key Lock" is displayed in first line.
8	Press the menu button (MENU).	MENU	MENU window is displayed. OK is already selected (displayed in white letters).
9	Press the enter key (ENTER).	ENTER	The set value is memorized, and top screen is displayed.

Procedures of Key Unlock (Changing Key Lock setting from 1(Lock) to 0(Unlock)).

	Operation	Key	LCD Display
1		----	Top screen is displayed.
2	Press the menu button (MENU).	MENU	MENU window is displayed.
3	Select Std-by in MENU window pressing the shift key (downward).	▼	Std-by is displayed in white letters.
4	Press the enter key (ENTER).	ENTER	Stand-by Setting screen is displayed and chamber temperature setting value is changed into white letters.
5	Select Key Lock item pressing Shift keys.	▼	Set value of (Key Lock) is displayed in white letters.
6	Change the value from 1 to 0 pressing the character input key.	0	Set value "0" is displayed.
7	Press the enter key (ENTER).	ENTER	Item of (Password) is displayed.
8	Set the password pressing the character input key.	0 0 0 0	The password **** is displayed.
9	Press the enter key (ENTER).	ENTER	The value of top item (Temperature) is displayed in white letters. "Key Lock" in first line is disappeared.
10	Press the menu button (MENU).	MENU	MENU window is displayed. OK is already selected (displayed in white letters).
11	Press the enter key (ENTER).	ENTER	The set value is memorized, and top screen is displayed.

Note: Consult our sales representative or agent if you put off the password.

HIGH LIMIT/LOW LIMIT ALARM (MENU/Std-by)

A high limit temperature alarm and low limit temperature alarm are provided with this product. The alarm temperature can be changed as follows:

1. With the top screen displayed, press the menu button (MENU) to show the menu window. Select "Std-by" and press the enter key (ENTER).

Stand-by Top Screen		MENU
Temp 25.0 °C	Alarm : Nor	Run
25.0 °C	Door : Clo	Std-by
	Light : OFF	Edit
2010/01/01	12:00:00	Tools
		M. Def

2. Stand-by Setting screen is displayed.

Stand-by Setting	
Temperature	25.0 °C (-10.0 °C - +60.0 °C)
Light Step	0 LS (0. OFF 1. ON)
Key Lock	0 (0. UnLock 1. Lock)
High Limit	65 °C
Low Limit	-15 °C

3. Set the desired high limit temperature alarm by turning the high limit temperature alarm volume (HIGH LIMIT) at the center of the control panel by using a small screw driver. The settable alarm temperature is between 15.0 °C and 65.0 °C.

Note:

Set the high limit temperature alarm (High Limit) 5 °C or higher than the maximum temperature in a program or stand-by operation.

4. Set the desired low limit temperature alarm by turning the low limit temperature alarm volume (LOW LIMIT) at the center of the control panel by using a small screw driver. The settable alarm temperature is between -15.0 °C and 20.0 °C.

Note:

Set the low limit temperature alarm (Low Limit) 5 °C or lower than the minimum temperature in a program or stand-by operation.

5. Press the menu button (MENU) at the completion of setting. The menu window is shown. Select "OK" and press the enter key (ENTER). The alarm temperature is memorized.

Refer to alarms and safety functions of page 46 for details.

Note:

High limit temperature alarm (High Limit) and low limit temperature alarm (Low Limit) are effective during a programmed running as well.

At any time when Stand-by Setting screen is not displayed, turning the high and low limit temperature alarm volume (HIGH LIMIT or LOW LIMIT) causes change of the setting value.

To avoid unexpected alarm depending on the ambient temperature or current running status, set High Limit or Low Limit temperature after actual temperature of chamber reaches to the set temperature of operation.

PROGRAMMING (MENU/Edit)

This product has two modes, which are clock mode and timer mode. The clock mode is used to set a change time to the next step in a day time (24 hours). The timer mode is used to set a time for each step directly and the remaining time is displayed.

The selection of either mode is available on the running mode selection screen at the start of the program.


Example 1:

Following shows the procedure to create a new program "Oze" of which cycle is 31 with clock mode.


The details of "Oze" is as follows:

Start time (H)	6:00	9:00	11:00	13:00	15:00	17:00	19:00	21:00	22:00	23:00	6:00
Temp (°C)		12	15	20	25	20	18	15	15	12	10
Lighting		0	1	0	1	0	1	0	1	0	1


1. With the top screen displayed, press the menu button (MENU) to show the menu window.

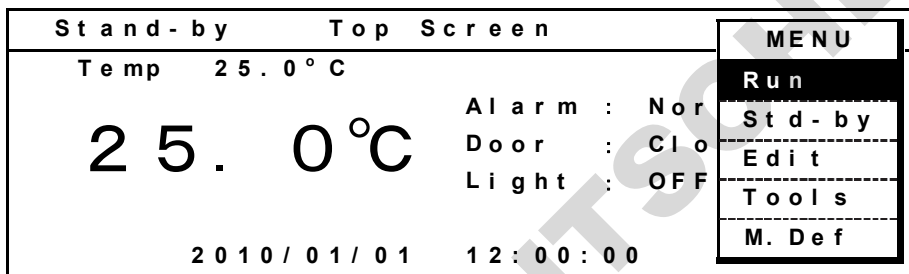


2. Select "Edit" and push the enter key (ENTER).

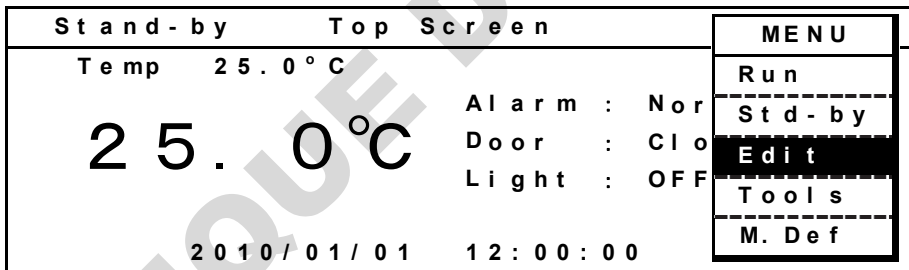


3. The Program Name Stored screen is opened. Press the menu button (MENU) and select "New" and press the enter key (ENTER). The program names are displayed when some programs have already been saved.

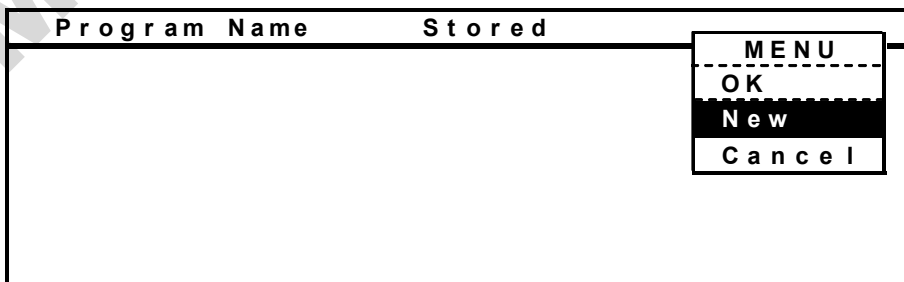

4. A model program is displayed.

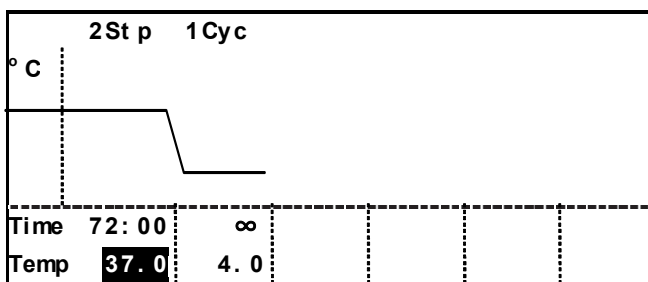

The step number (Stp :step) and cycle number (Cyc :repeat number) can be changed on the top left corner (2 Stp 1 Cyc) of the screen. Highlight the numerical value by shift key and input 10 Stp 31 Cyc by character input key. The step number and cycle number are changed. The screen is scrolled to the next page by using the rightward shift key.

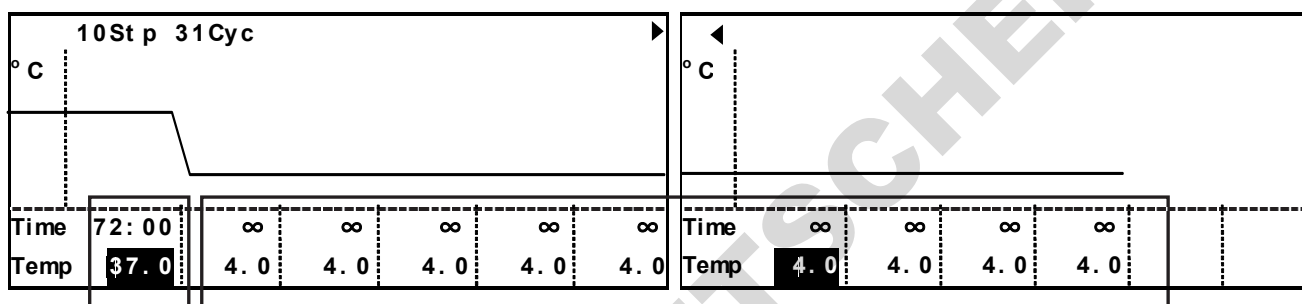

MENU

Save
+ / -
Cancel


MENU

Save
Insert
Delete
+ / -
Cancel

The step number (Spt) can be changed by "Insert" or "Delete" on the menu window. Press the menu button (MENU), to open the menu window. The menu window for a first section has no "Insert" or "Delete". Therefore, neither insert nor delete is effective for the first section. The maximum step number is 12. The cycle number is 1 when the step number is 1. The settable cycle number is up to 98. The cycle number 99 means limitless repeat.

PROGRAMMING (MENU/Edit)


5. Highlight the numerical value of each time section (Time) by shift key, and input as below by character input key.

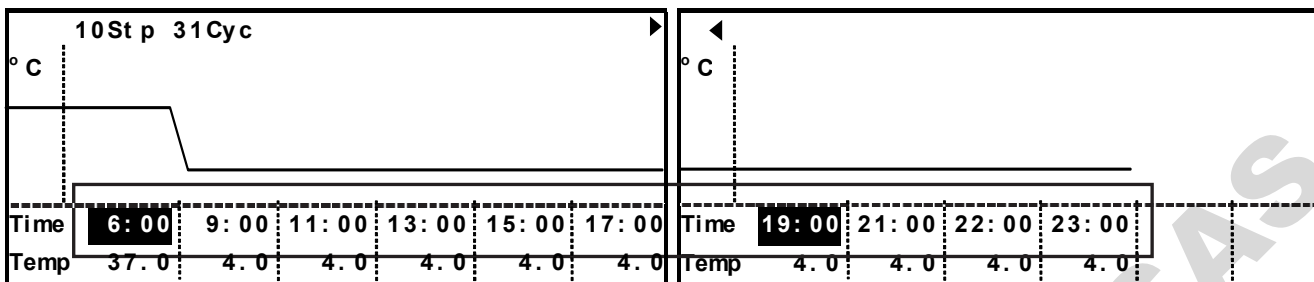

CAUTION

The time setting value depends on each mode, clock mode and timer mode. In the case of clock mode, the setting range is between 00:00 and 23:59. If the setting is larger than 24:00, the step of immediately before is repeated limitlessly. Set the step with timer order. If an earlier time than the previous step is inputted, the previous step is skipped. In the case of timer mode, setting range is between 00:01 and 99:59. The setting of "99:99" causes limitless repeat.

6. Shift a cursor downward by the downward shift key. Set the temperature as follows. The setting range is between -10.0 °C and +60.0 °C.

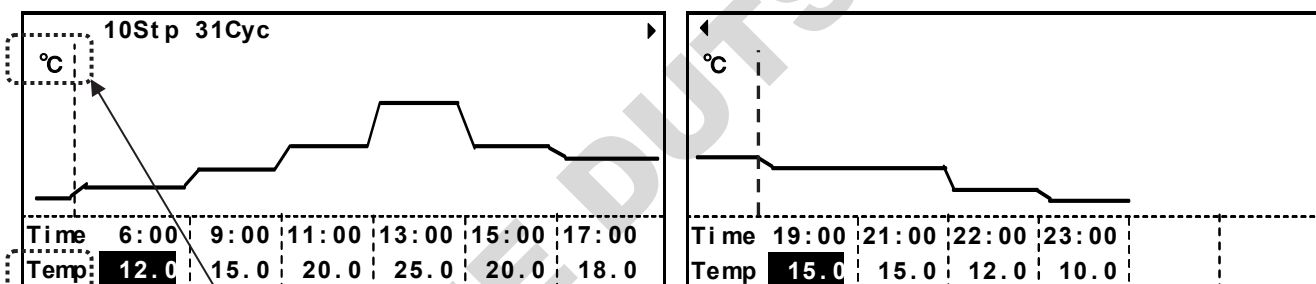

During temperature setting, "°C" is displayed at upper left.

MENU
Save
+ / -
Cancel

When adding the "-" to the set value of temperature or erasing the "-" from the set value of temperature, press the menu button (MENU) to show the menu window. Select +/- and press the enter key (ENTER).

CAUTION


The settable range of chamber temperature is between -10 °C and +60 °C.

- The lighting is available only with temperature range between +2 °C and +50 °C when the optional light add on kit (MIR-L15) is installed. In the case of temperature out of range, the lighting is not usable. The lamp is off with the temperature out of range when the saved program is running. In this case, temperature fluctuation may exceed ± 1.5 °C or it may take longer time to pull down the chamber temperature.
- The temperature control range is -10 °C~+50 °C when the optional inner door (MIR-55ID) is installed. The temperature is limited to 50 °C when the saved program includes temperature setting over 50 °C. In this case, the temperature setting over 50 °C is indicated by blinking.

CAUTION


The unit continues to run with a step just before the step having time setting of over 24:00 when a program is run in clock mode.

7. Shifting a cursor downward by downward shift key moves to the next edit "Light" (light step).

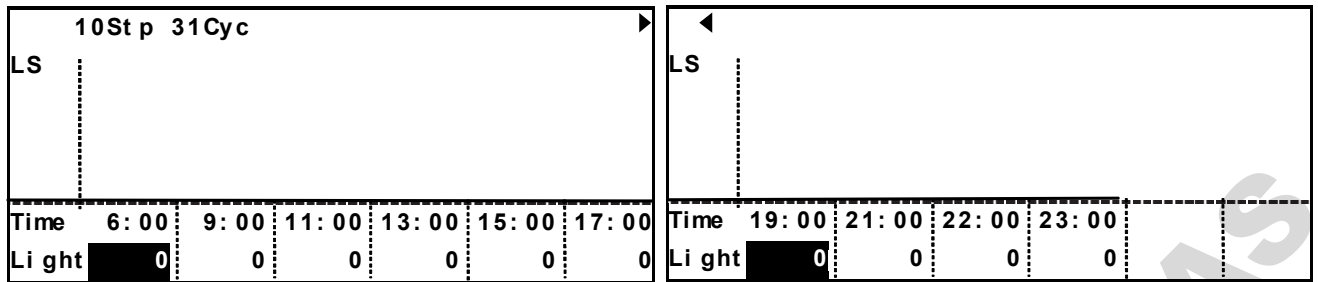


Set a light step as below. To set 0(OFF) or 1(ON).

· Light step can set only the temperature range between +2 °C and +50 °C to 1(ON), when the optional light add on kit (MIR-L15) is installed.

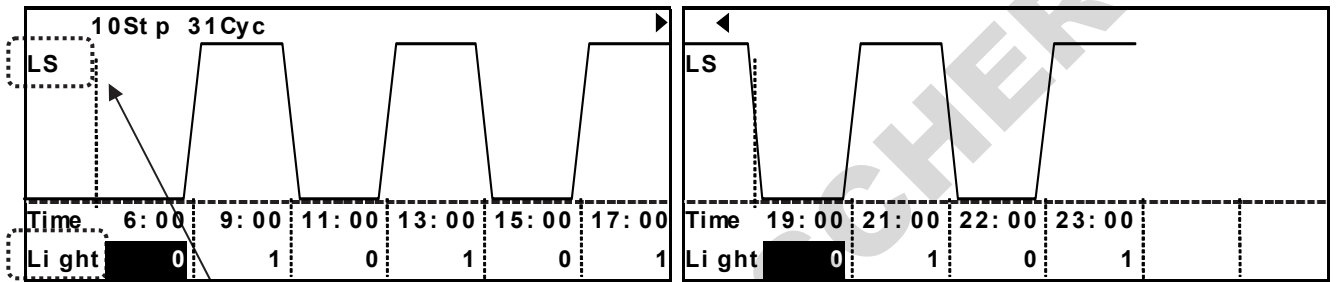


When setting Light step, "LS" displayed at the upper left and "Light" at the lower left on the top screen.

8. Shifting a cursor downward by downward shift key moves to the next edit "Temp" (Temperature).

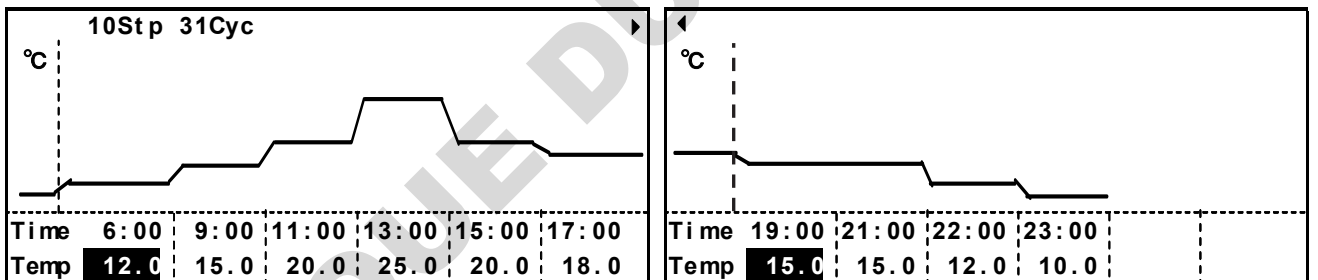


9. At the completion of all input, press the menu button (MENU) to show the menu window. Select "Save" and press the enter key (ENTER). Save Program screen is opened.

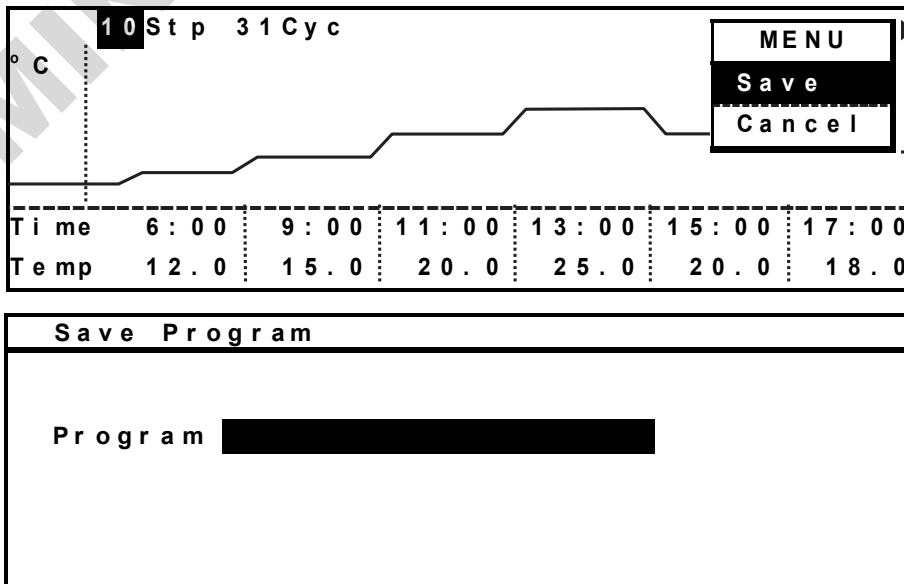

PROGRAMMING (MENU/Edit)

10. Input a program name (Oze) and press the menu button (MENU) to show the menu window. Select "Save As" and press the enter key (ENTER). The program is entered. The maximum numbers of character for program name is 16. Refer to edit function of characters described below. Up to 10 programs are created and saved.

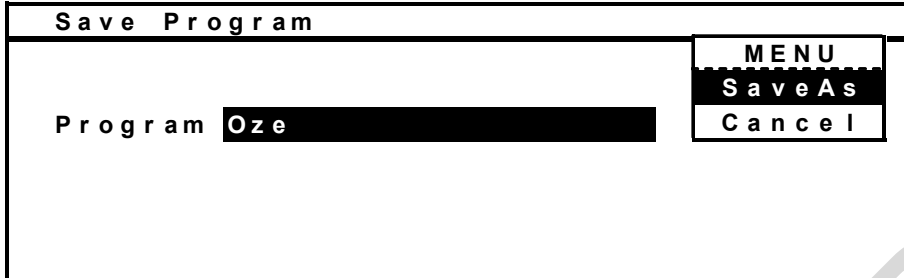

Edit function of characters

Shift key

- **Upward shift key:** Space insertion
- **Downward shift key:** backspace
- **Leftward shift key:** Move a cursor left
- **Rightward shift key:** Move a cursor right

Character input key

- | | | | |
|---------------------------------|-----------------------------|---------------------------------|----------------------------|
| 1 key: space,-,"#, @,1 | 2 key: A,B,C,a,b,c,2 | 3 key: D,E,F,d,e,f,3 | |
| 4 key: G,H,I,g,h,i,4 | 5 key: J,K,L,j,k,l,5 | 6 key: M,N,O,m,n,o,6 | |
| 7 key: P,Q,R,S,p,q,r,s,7 | 8 key: T,U,V,t,u,v,8 | 9 key: W,X,Y,Z,w,x,y,z,9 | 0 key: &,/, (,),.,0 |


11. Return to the top screen after saving program.

Example 2:



To create the following program with timer mode and name "NIKKO". The cycle is 99, that is limitless repeat.

Step Time	48	36
Temperature (°C)	20	30
Light Step	0	1



1. Display a model program as shown on page 22.

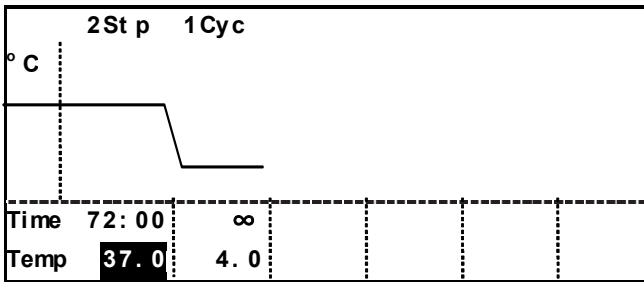

Change the step number and cycle number to 2 Stp and 99 Cyc by character input key. Only one page is displayed and 99 is changed into ∞. Display of ∞ changes 99 when lapped by a cursor.

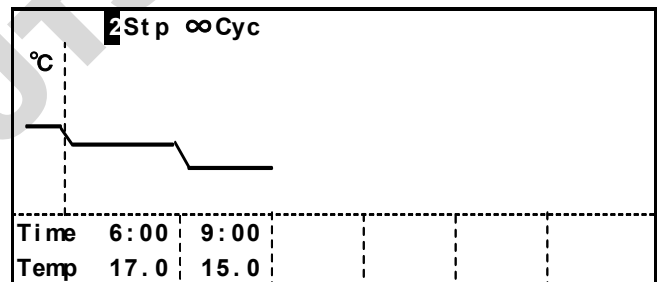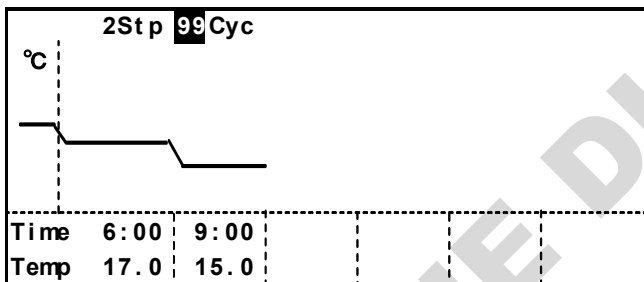


2. Set a time, temperature and light step as same as Example.1.

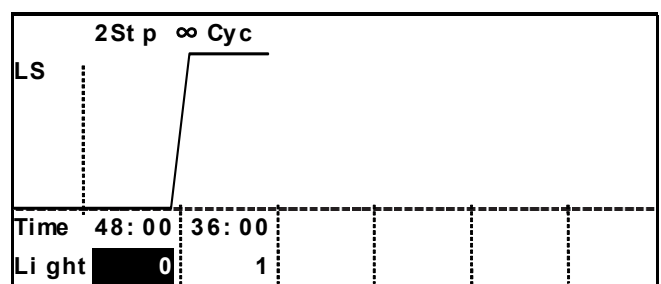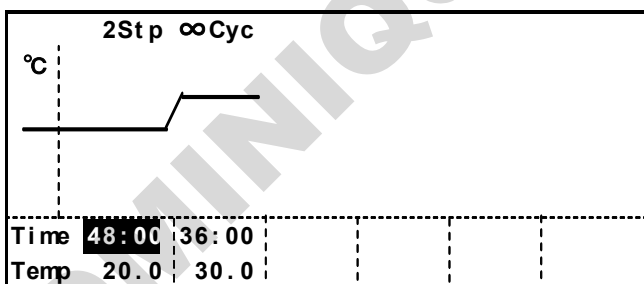

3. Input a program name (NIKKO), press the menu button (MENU) to show the menu window. Select "Save As" and press the enter key (ENTER) to save the program as same as Example.1.

EDIT OF SAVED PROGRAM (MENU/Edit)


1. With the top screen displayed, press the menu button (MENU) to show the menu window. Select "Edit" and press the enter key (ENTER).

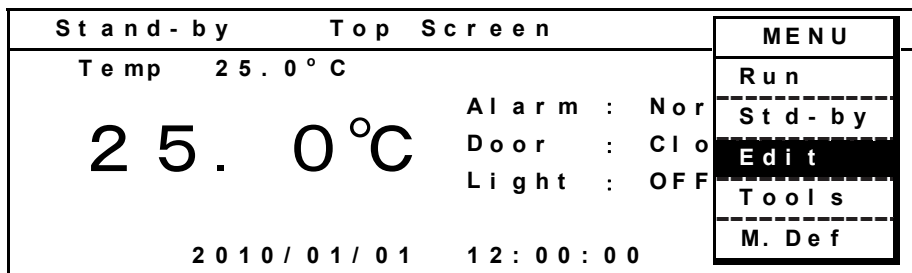

2. The saved programs are shown. Select a program (for example: Oze) to edit and press the menu button (MENU). The menu window is opened. Select "OK" and press the enter key (ENTER).



3. The program "Oze" is displayed. After changing the setting, press the menu button (MENU) to show the menu window. Select "Save" and press the enter key (ENTER).

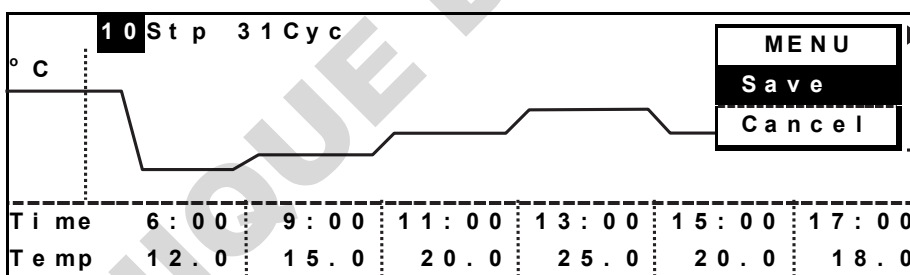

4. Save Program screen is opened. Input program name and press the menu button (MENU) to show the menu window. Select "Save" when saving by overwriting or select "SaveAs" when saving with another program name. Press the enter key (ENTER). The edited program is entered. Do not select "SaveAs" with same program name as another program.



START OF PROGRAM (MENU/Run)

1. With the top screen displayed, press the menu button (MENU) to show the menu window. Select "Run" and press the enter key (ENTER).

Stand-by		Top Screen		MENU	
Temp	25.0°C	Alarm	: Nor	Run	
25.0°C		Door	: Clo	Std-by	
		Light	: OFF	Edit	
2010/01/01		12:00:00		Tools	
				M. Def	

2. Program Name Stored screen is opened. Select "Oze" and press the menu button (MENU) when starting "Oze" program. Select "OK" on the menu window and press the enter key (ENTER).

Program Name	Stored	MENU	
Oze	10/01/01 12	OK	
NIKKO	10/01/01 12	Cancel	

3. Start Options screen is opened. On this screen, setting of Timer (selection of Clock mode or Timer mode), Join (Joining some programs), and start date is available. As the "Oze" is for clock mode, select 1 (Clock) for Timer. For join, select 2 (No : not join) since the Oze does not have joined program. Input the start date (Ex.2010 01 01) and time (Ex.12:30:00) and press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

Start Options	
Timer	1 (1. Clock 2. Dec)
Join	2 (1. Yes 2. No)
Start at	
Date	10/01/01 (YY/ MM/ DD)
Time	12:30:00 (hh: mm: ss)

■ Timer (selection of Clock mode or Timer mode)

1. Clock (Clock mode): Displays start time of each steps.
2. Dec (Timer mode): Displays the remaining time up to a next step.

■ Join (Joining some programs)


Join 1.Yes: The joined programs are operated when a selected program is set as a join program. Refer to page 31 for details.

■ Start at (desired start date)



Date and time when the window is opened is displayed. Input the desired start date and time.

START OF PROGRAM (MENU/Run)

4. The selected program is displayed. Check the program and press the menu button (MENU) to show the menu window. Select "Start" and press the enter key (ENTER).

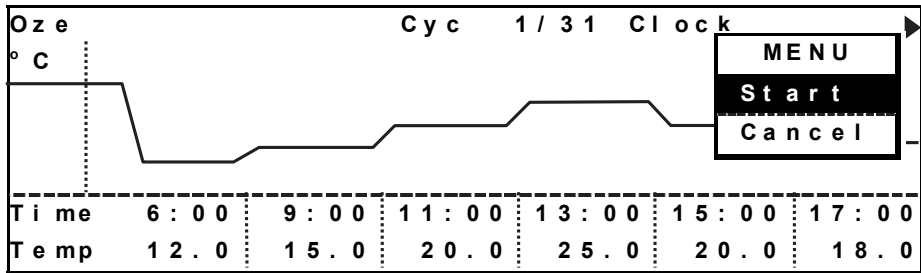

5. The program is started at desired date and time. During the programmed running, the graphic screen as below is displayed. To change the graphic screen to the top screen, press the menu button (MENU) to show the menu window. Select "Top" and press the enter key (ENTER). To change to the graphic screen, press the menu button (MENU) to show the menu window. Select "Graph" and press the enter key (ENTER).

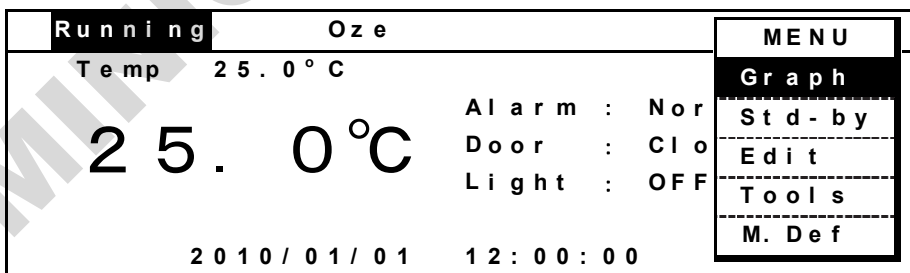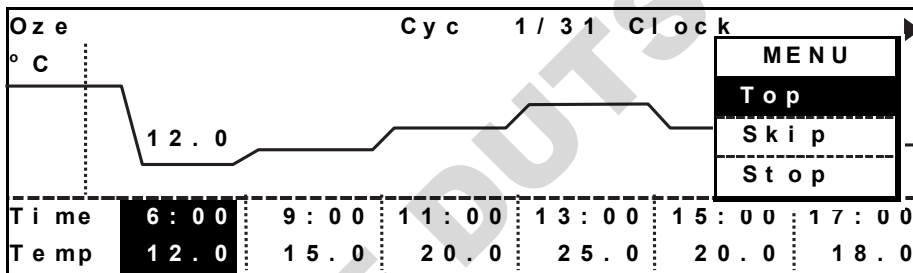

When the starting time of program operation is later, "Waiting" is displayed in the current running status of LCD panel.

JOIN FUNCTION

This product has join function to run several programs continuously. The maximum programs to be joined are 9. The setting of join function is as follows:

1. When joining three programs Spring, Summer and Autumn, input the same character string, # and one digit figure (joined order) before each program name. Each program operates as a special program for join function. Any character or figure is permitted for a string on the top. The programs cannot be joined when the character string is not same.

Note: The characters after one digit figure have no effect on the join function.

Ex.1: When joining the programs Spring, Summer and Autumn in this order and top character string is "Oze" the input for the join function is as follows:

Oze#1 Spring Oze#2 Summer Oze#3 Autumn

Ex.2: When joining in the order of Autumn, Spring and Summer in this order and input "NIKKO" as the same character string, the input for the join function is as follows:

NIKKO#1 Autumn NIKKO#2 Spring NIKKO#3 Summer

2. When running the joined program in Ex.1, select the program Oze#1 Spring on the Program Name Stored screen in MENU/Run (Refer to page 29).

Note: The program Oze#2 Summer is selected, the program Oze#2 Summer and Oze#3 Autumn are performed. Oze#1 Spring is not joined.


3. Select 1.Yes for the join function on the Start Options screen. Press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

Note: The joined function is not effective if select 2. No on the Start Options screen.

4. Press the menu button (MENU) to show the menu window. Select "Start" and press the enter key (ENTER). The joined program is started.

5. Running result


Run in the order of Oze#1 → Oze#2 → Oze#3. During the running of joined program, "Join" is displayed at the upper right on the screen.

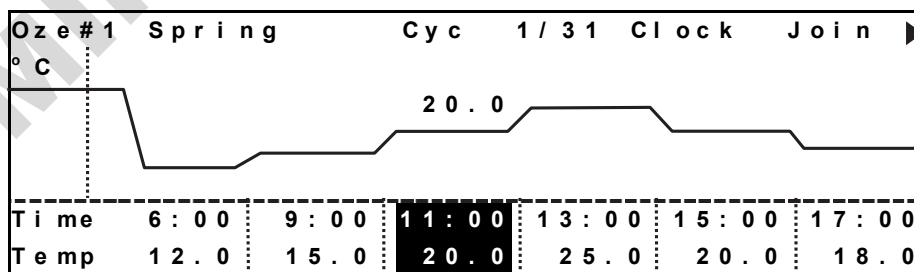

SKIP OF STEP (MENU/Skip)

During the programmed running, the skip function is effective to skip a current step in the program.


1. Press the menu button (MENU) to show the menu window and select "Graph" when the top screen is displayed. Then press the enter key (ENTER).
2. Press the menu button (MENU) under program running and the menu window is opened. Select "Skip" and press the enter key (ENTER).

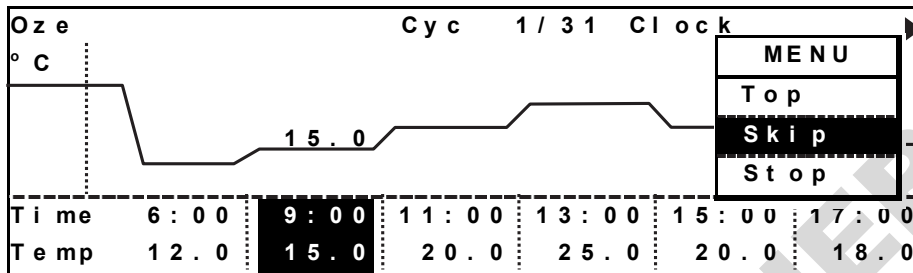

3. The Confirmation screen is displayed. Press the menu button (MENU). Selecting "Next" causes the skip to the next step. Selecting "Back" causes the skip to the previous step. After selecting "Next" or "Back", press the enter key (ENTER).




4. Programmed running shifts to next step and programmed running continues.

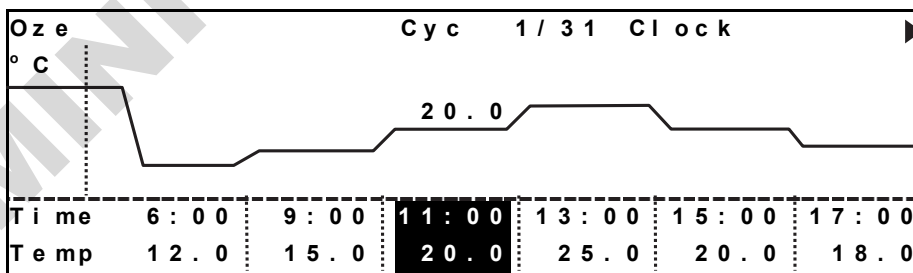


STOP OF PROGRAM (MENU/Stop)

During the programmed running, it is possible to stop the running at any step.


1. During the programmed running, press the menu button (MENU) to show the menu window and select "Graph" when the top screen is displayed. Then press the enter key (ENTER).
2. Press the menu button (MENU) under program running and the menu window is opened. Select "Stop" and press the enter key (ENTER).

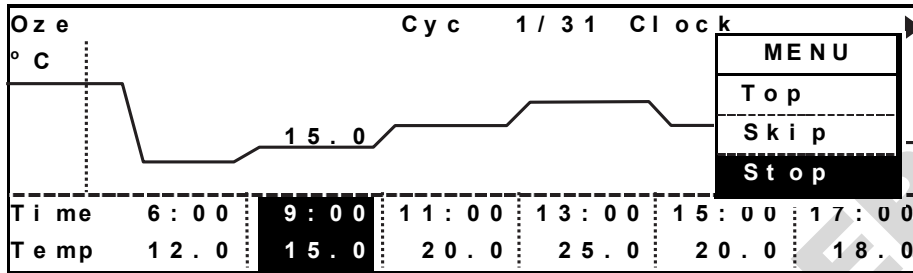

3. The Confirmation screen is displayed. Select "OK" and press the enter key (ENTER) to stop the program.

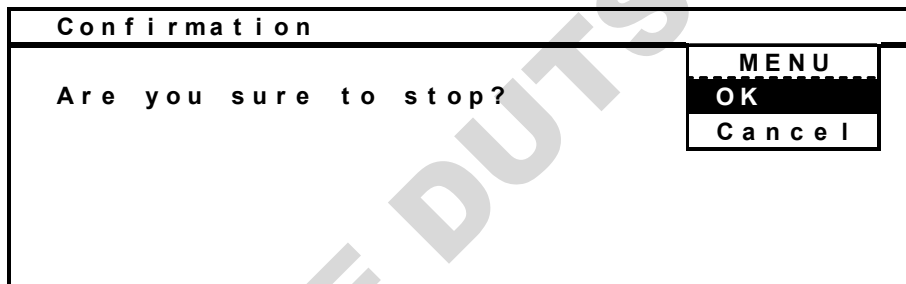


4. After stopping the program, the top screen is displayed.

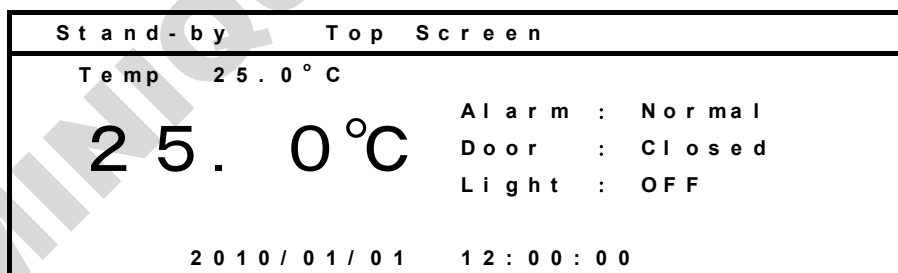


AUTOMATIC DEFROST (MENU/Tools/Date Time)

This product has a frost check opening to check amount of the frost on the evaporator that lowers temperature in a chamber. Automatic defrost function defrosts the frost on the evaporators automatically at the specified time everyday. Default setting is 0(Manual).

1. Press the menu button (MENU) to show the menu window and select "Tools" when the top screen is displayed. Then press the enter key (ENTER).
2. Select "Date Time" on the Select Tools screen and press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

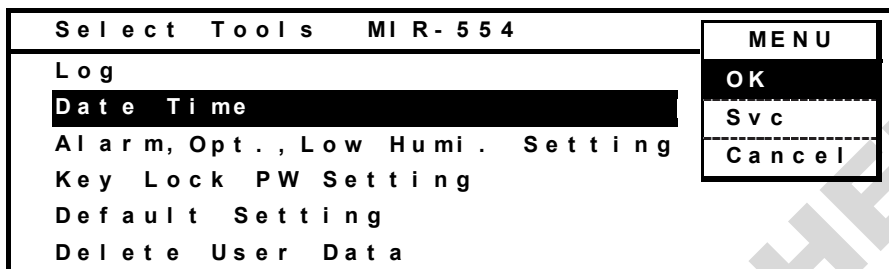

3. The Date Time screen is displayed. Select the Def Timer (Automatic defrost function) 0 (Manual) or 1 (Auto). When selecting 0 (Manual), automatic defrosting is not done. When selecting 1 (Auto), it is possible to set the time to defrost automatically in every one hour between 0:00 and 23:00. (The figure below shows that the defrost starts at 3:00.)

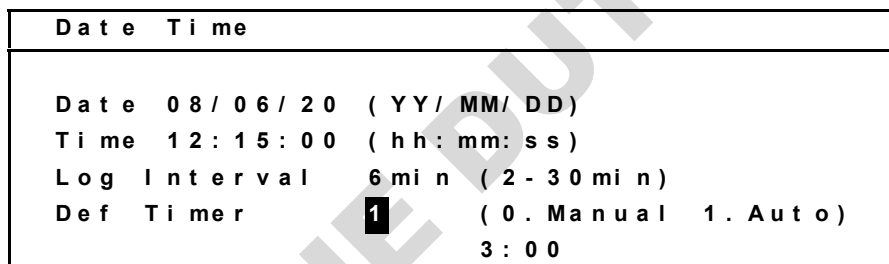

⚠ CAUTION

Automatic defrosting is activated even in programmed running, and the chamber temperature may arise due to the amount of the frost existing on the evaporator. In this case, manual defrosting is recommended.

⚠ CAUTION

During defrosting, "Defrosting" is displayed on running status of LCD panel.

During defrosting, the chamber temperature deviates from the set temperature (The chamber temperature raise by approximately 2 °C with the setting temperature of 5 °C under ambient temperature of 30 °C and humidity of 80 %R.H.)

Care should be taken for deviation of setting and current temperature during defrosting. In case of long term running of setting temperature below 5 °C, expected running will be failed due to frost.


Defrosted water will be evaporated automatically outside of the chamber.

- Defrosting is likely not to operate when the inner temperature is over 5 °C.
- Frost will exist on the evaporator when temperature setting is below 5 °C. Frost-clogged evaporator causes insufficient cooling and inner temperature rising. When a lot of frost existed on the evaporator is seen through the frost check opening, immediate defrosting is required. Frosting on the evaporator is accelerated when moisturized material is put inside the chamber.


MANUAL DEFROST (MENU/M.def)

The manual defrost function is for defrosting the frost on the evaporator at any time. When a lot of frost on the evaporator is found, start the manual defrost. Besides this function, it is possible to set the automatic defrost function. (Refer to page 34)


1. Press the menu button (MENU) to show the menu window. Select "M.Def" and press the enter key (ENTER).

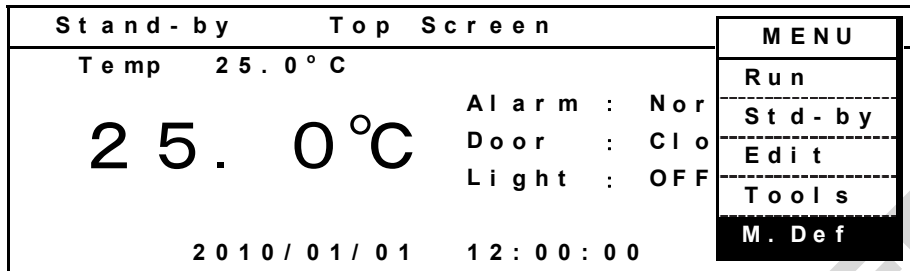

2. The Confirmation screen is displayed.

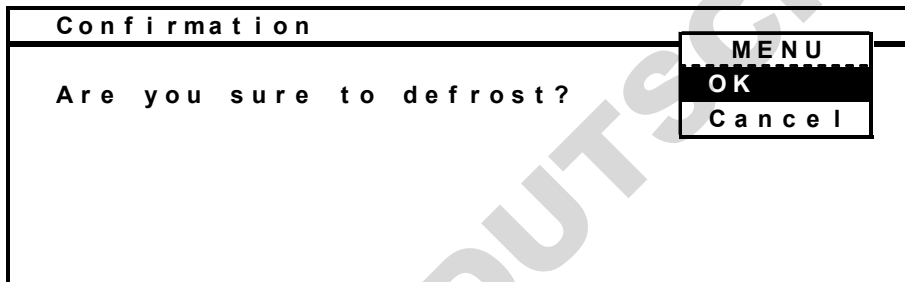

3. Select "OK" and press the enter key (ENTER). The manual defrost is started. During defrosting, "Defrosting" is displayed at the upper left on the top screen.

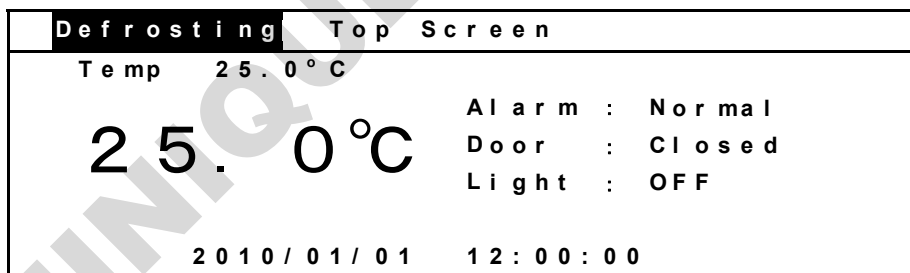

CAUTION


The manual defrost can be started during programmed running, standby operation, or automatic defrosting.

4. The manual defrost is finished automatically. The defrosting time depends on the amount of frost on the evaporator.


VARIOUS SETTING (MENU/Tools)

The log can be displayed, and various setting can be changed by using "Tools" menu.

1. Press the menu button (MENU) with the top screen to show the menu window. Select "Tools" and press the enter key (ENTER).

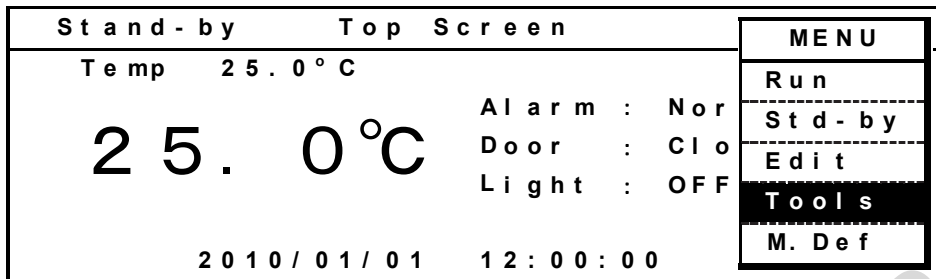


2. The Select Tools screen is as follows.

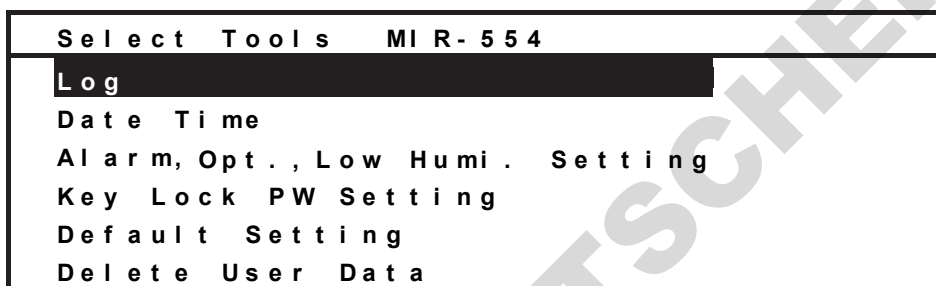

Display of log (Tools/Log)



1. Select "Log" in the Select Tools screen. Press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

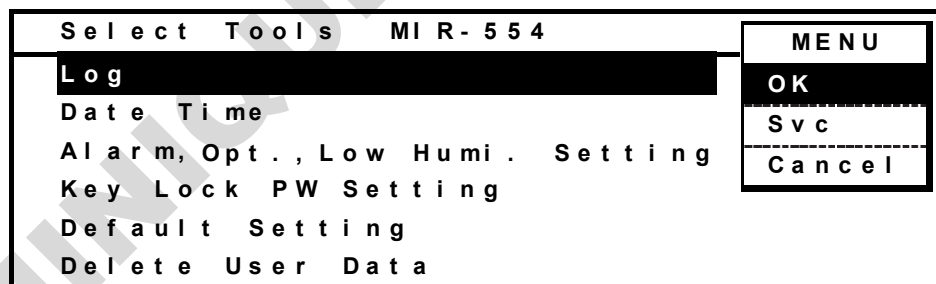



2. The log is presented with dot. By pressing the upward shift key or downward shift key, the log to be displayed is changed; temperature and light step. The displayed date is scrolled by pressing the leftward or rightward shift key. (leftward shift key; older date, rightward shift key; newer date.)



3. The display area (upper and lower limit) can be changed. Press the menu button (MENU) to show the menu window. Select "Range2" and press the enter key (ENTER). Upper limit is changed from 50 °C to 60 °C and lower limit is changed from 0 °C to -10 °C.

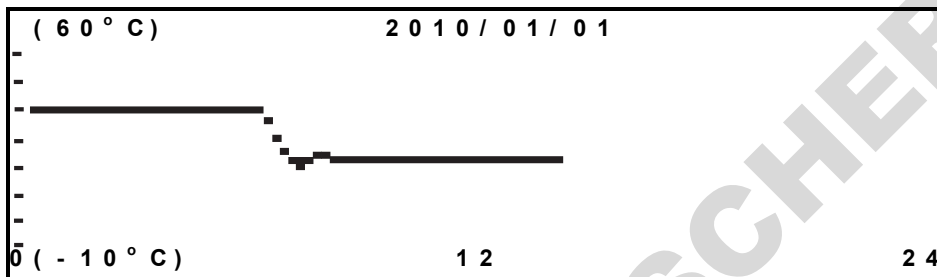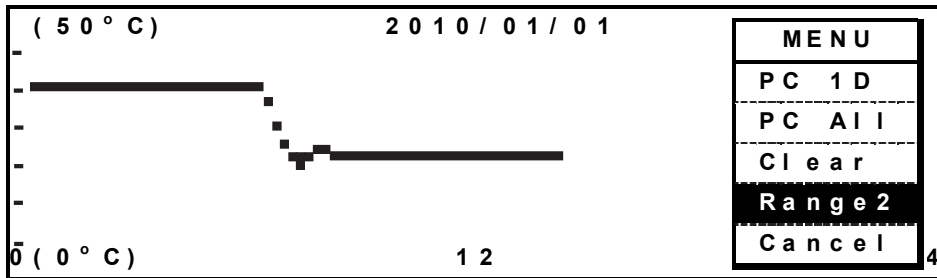

Similarly, select "Range1" and press the enter key (ENTER). Upper limit is changed from 60 °C to 50 °C and lower limit is changed from -10 °C to 0 °C.

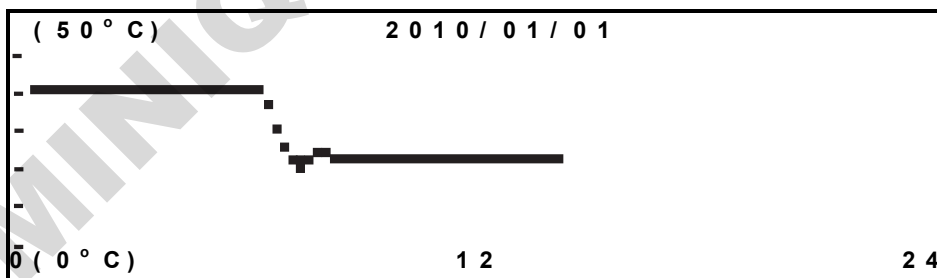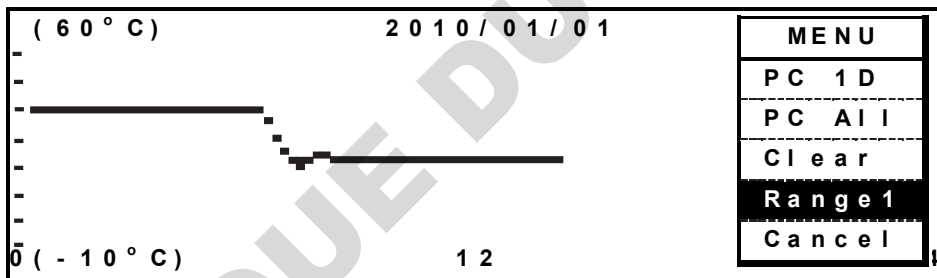


VARIOUS SETTING (MENU/Tools)


Data transmission

The procedure to transmit the log data to a PC is as follows.

1. Press the menu button (MENU) to show the menu window. Select "PC 1D" and press the enter key (ENTER) when the log for one day is necessary. Select "PC All" and press the enter key (ENTER) when all data recorded is necessary.

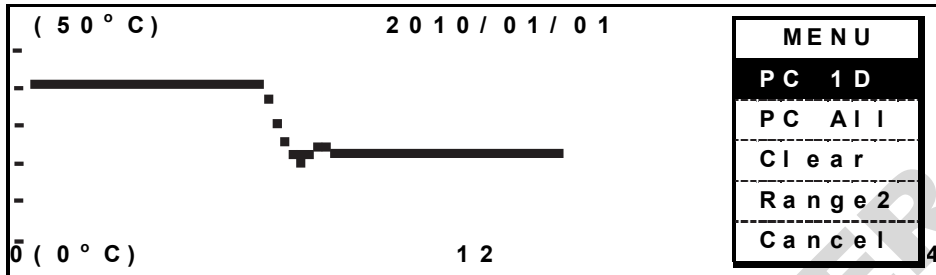

2. The Progress screen is displayed. Specify a transfer, capture of text and retention file name by operation of hyper terminal on PC. Apply "txt" or "csy" to retention file as an extension. Press the menu button (MENU) to show the menu window. Select "Start" and press the enter key (ENTER). The transmission is started. "Finished" display means the end of transmission.

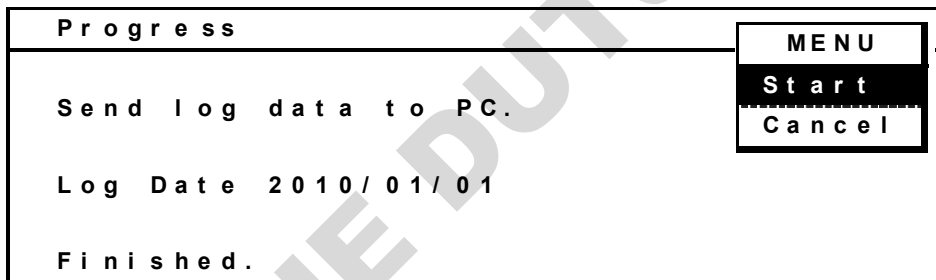

Setting in PC side for transmission of log data

As for setting in PC side for transmission of log data, please contact our sales representative or agent.

Setting of date, time, log (Tools/Date Time)

1. Select "Date Time" in the Select Tools screen. Press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

Select Tools	MIR-554				
Log	<table border="1"> <tr><th>MENU</th></tr> <tr><td>OK</td></tr> <tr><td>Svc</td></tr> <tr><td>Cancel</td></tr> </table>	MENU	OK	Svc	Cancel
MENU					
OK					
Svc					
Cancel					
Date Time					
Alarm, Opt., Low Humi. Setting					
Key Lock PW Setting					
Default Setting					
Delete User Data					

2. The Date Time screen is displayed. Set date, time or log cycle.

Date Time	
Date	10/01/01 (YY/MM/DD)
Time	12:00:00 (hh:mm:ss)
Log Interval	6 min (2-30 min)
Def Timer	1 (0. Manual 1. Auto)
	3:00

- Date input (Ex: Feb. 14, 2010)
Input 100214 in the date cell.

- Time input (Ex: 12:15:00)
Input 121500 in the time cell.

- Log cycle input (Ex: 6 minutes)
Input 6 in log Interval cell.

Notes:

- The default is 6 minutes.
- The acceptable range is between 2 and 30 minutes.
- Relation between the log interval and spans that can be memorized

1: Log interval 2 min	About 5 days
2: Log interval 6 min	About 14 days
3: Log interval 30 min	About 70 days

After passing the memory limit, the older data is deleted, and newer data is memorized.

- Setting of automatic defrost

Select one of two defrosting patterns. The default is 0(Manual defrost). For the details of defrost, refer to page 34~35.


0: Manual defrost

1: Automatic defrost

VARIOUS SETTING (MENU/Tools)

Alarm setting (Tools/Alarm, Opt., Low Humi. Setting)

1. Select "Alarm, Opt., Low Humi. Setting" in the Select Tools screen. Press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

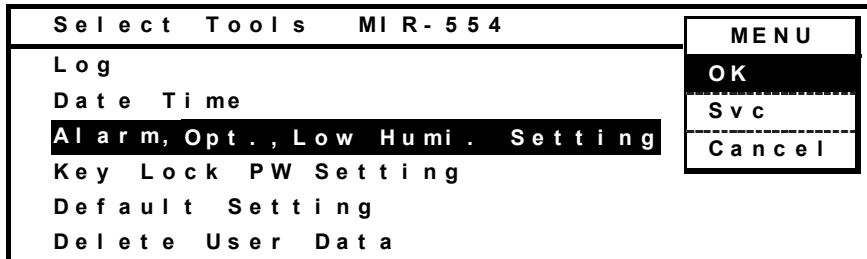

2. The Alarm, Option, Low Humidity Setting screen is displayed. On this screen, the temperature alarm (Temp Alarm), delay time of alarm (Alarm Delay), alarm resume time (Ring Back) and lamp (Lamp) can be set. The alarm buzzer is silenced by pressing the alarm buzzer stop key (BUZZER) during alarm condition. The buzzer will be activated again after certain suspension if the alarm condition continues. The suspension time (ring back) can be set.

Alarm, Option, Low Humidity Setting	
Temp Alarm	± 2.5 °C (± 1.0 °C - ± 5.0 °C)
Alarm Delay	15 min (0 - 15 min)
Ring Back	30 min (0. OFF 1 - 99 min)
Inner Door	0 (0. Normal 1. Option)
Lamp	0 (0. Normal 1. Option)
Low Humidity Mode	0 (0. No 1. Yes)

The settable range:

- Temperature alarm (Temp Alarm): ±1.0°C~±5.0°C.
- Delay time of alarm (Alarm Delay): 0 minute~15 minutes.
- Suspension time (Ring Back): 1 minute~99 minutes, or OFF

3. When optional inner door (MIR-55ID) is installed, set the inner door (Inner Door) to 1.

- When the inner door is installed, the set temperature is limited under 50 °C.
- The inner door might be damaged by running at the temperature that exceeds 50 °C as the setting of the inner door (Inner Door) is 0.

4. When optional light add on kit (MIR-L15) is installed, set the lamp (Lamp) to 1.

- When optional light add on kit (MIR-L15) is installed, except when the set value of temperature is between +2 °C~+50 °C, the lighting is turned off. The set value of temperature is limited between +2 °C~+50 °C after Lamp is set to 1.

5. The condensation in the chamber is reduced by running control with the set temperature between +20 °C and +40 °C when the low humidity mode (Low Humidity Mode) is set to 1.

- The condensation can be found on the inside of the door or clearance in the chamber when running in humid chamber status without low humidity mode (Low Humidity Mode is set to 0).

CAUTION

It is not possible to change the delay time of door alarm, 2 minutes only. When door is open, "Open" is displayed on the top screen.

Key lock password setting (Tools/Key Lock PW Setting)

1. Select "Key Lock PW Setting" in the Select Tools screen. Press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

Select Tools M I R - 5 5 4	MENU
Log	OK
Date Time	Svc
Alarm, Opt., Low Humi. Setting	Cancel
Key Lock PW Setting	
Default Setting	
Delete User Data	

2. Input the Current User Password (4 digits) and press the enter key (ENTER).
The default User Password when shipped from the factory is "0000".

Key Lock PW Setting
Current User Password <input type="password"/>

3. Input New User Password (4 digits) and press the enter key (ENTER).

Key Lock PW Setting
New User Password <input type="password"/>

4. Input User Password (4 digits) again and press the enter key (ENTER).

Key Lock PW Setting
New User Password ****
Re Enter User Password <input type="password"/>

Note: Consult our sales representative or agent if you put off the password.

VARIOUS SETTING (MENU/Tools)

Default setting (Tools/Default Setting)

1. Select "Default Setting" in the Select Tools screen. Press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

Select Tools	MIR-554
Log	MENU OK Svc Cancel
Date Time	
Alarm, Opt., Low Humi. Setting	
Key Lock PW Setting	
Default Setting	
Delete User Data	

2. The Default Setting screen is displayed. Set the default for each parameter as necessary.

Default Setting		
LCD Back Color	1	(1. Blue 2. White)
DAQ Speed	0	(0. 2400 2. 9600)
DAQ ID	0	(0. OFF 1- 250)
DAQ Mode	0	(0. Local 1. Remote)
Buzzer Finished	1	(1. Yes 2. No)
Analog Range	0	(0. Normal 1. Wide)

LCD Back Color: Setting of background color (1. Blue 2. White)

Buzzer Finished: Select of buzzer activation (1: Yes) or no activation (2: No) at the time of completion of a programmed running. (The buzzer activates 6 times when a program is finished.)

Analog Range: Select of analog output range of temperature in chamber (0: 0°C~50°C 1: -20°C~80°C)

Note:

DAQ is an external monitoring system of chamber status. It is necessary to set the DAQ Speed, DAQ ID and DAQ Mode when using communication software. Communication software is ordered specially consult our sales representative or agent.

Delete of program (Tools/Delete User Data)

1. Select "Delete User Data" in the Select Tools screen. Press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

Select Tools	MIR-554	MENU
Log		OK
Date Time		Svc
Alarm, Opt., Low Humi. Setting		Cancel
Key Lock PW Setting		
Default Setting		
Delete User Data		

2. The Delete User Data screen is displayed. To select a program to delete, select "Delete a User Program" and press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).

Delete User Data	MENU
Delete a User Program	OK
Delete All User Programs	Cancel

3. A list of saved programs is displayed. Select a program (Ex: Oze#1 Spring) to delete, press the menu button (MENU) to show the menu window. Select "Delete" and press the enter key (ENTER).

Program Name	Stored	MENU
Hatsuga	10/01/18 15	Delete
Oze#1 Spring	10/01/18 16	Cancel
Oze#2 Summer	10/01/18 20	
Oze#3 Autumn	10/01/18 21:45:00	

4. The Confirmation screen is displayed. Press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER). The program (Oze#1 Spring) is now deleted.

Confirmation	MENU
Are you sure to Delete?	OK
Program name Oze#1 Spring	Cancel

VARIOUS SETTING (MENU/Tools)

5. To delete all programs, select "Delete All User Programs" in Delete User Data screen and press the menu button (MENU) to show the menu window. Select "OK" and press the enter key (ENTER).


Delete User Data	
Delete a User Program	MENU OK Cancel
Delete All User Programs	

6. The Confirmation screen is displayed. The menu window is already displayed. Select "OK" and press the enter key (ENTER). All of the programs are now deleted.

Confirmation	
Are you sure to delete	MENU OK Cancel
All User Programs?	

ADJUSTMENT OF SHELVES

The interval between the shelves can be adjusted depending on the height of the stored items. To install the shelves, insert the clip to the desired location.

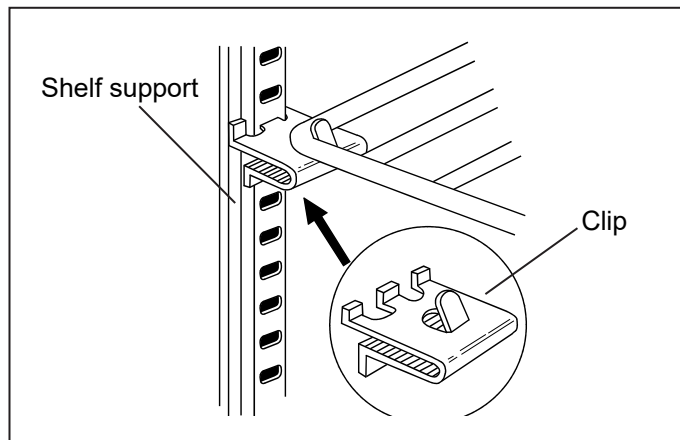

Notes:

- The chamber is refrigerated by the forced circulation of cooled air inside the chamber. Ensure that the intake and exhaust vents are not blocked. Blocking these vents cause deviation of chamber temperature from the set temperature.
- Always install the stainless plate on the bottom shelf. The operation without this plate makes the temperature distribution worse.
- Do not store any materials that can generate the corrosive gas such as sulfureted gas or gaseous chlorine in the chamber. The corrosive gas may cause failure of the products.

ALARMS AND SAFETY FUNCTIONS

The unit has the alarms and safety function as shown in the table 1 below.

Table 1 Alarms and safety functions


Alarm	Condition	Display	Buzzer	Remote contact	Safety operation
Auto-set temp. alarm	When the chamber temp. deviates from set temp. by more than 2.5 °C. (± 1.0 °C~5.0 °C changeable)	<Top screen> The current chamber temp. blinks.	Intermittent tone with delay	Alarm status with delay	---
Upper limit alarm	When the chamber temp. is higher than the upper limit temp.	----	Continuous tone	Alarm status	Heater, lamp OFF
Lower limit alarm	When the chamber temp. is lower than the lower limit temp.	----	Continuous tone	Alarm status	Compressor OFF
Thermal fuse	When the chamber temp. is over 70 °C	----	---	—	Main heater and sub-heater OFF
Thermal sensor abnormality	Input voltage is over 70 °C corresponding Input voltage is lower than -50 °C corresponding	<Top screen> “E01:Temp. sensor is opened.” “E02:Temp. sensor is shorted.”	Intermittent tone	Alarm status	Heater, lamp, fan motor and compressor OFF
Short-circuit of SSR or compressor relay	Microcomputer determines triac/compressor relay is shorted	<Top screen> “E04:SSR or comp. relay is shorted.”	Intermittent tone	Alarm status	---
Disconnection of SSR	The heater is not energized	<Top screen> “E05:SSR is open-circuited.”	Intermittent tone	Alarm status	---
Disconnection of compressor relay	The compressor relay is not energized	<Top screen> “E06:Comp. relay is open-circuited.”	Intermittent tone	Alarm status	---
Buzzer delay	Under condition of auto-set temp. alarm (delay time; changeable)	----	---	—	---
Back-up of program	During power failure	----	---	—	Nonvolatile memory Continuous running after recovery from power failure

Alarm	Condition	Display	Buzzer	Remote contact	Safety operation
Back-up of clock function	During power failure	----	---	—	Continuous running by battery (CR2032)
Fan lock	Fan is locked	<Top screen> “E07:Air circulating fan motor trouble.”	Intermittent tone	Alarm status	Compressor OFF and heater OFF
Protection of compressor	The protective sensor is higher than 90 °C	<Top screen> “E08:Comp. is over-heat.”	Intermittent tone	Alarm status	----
Time to replace the fan motor	The running time is over 60,000 hours	<Top screen> “Warning:Replace air circulating fan mot.”	---	—	---
Disconnection of compressor protective sensor	The input voltage corresponds to -50 °C or less disconnection of sensor	<Top screen> “E09:Comp.sensor is opened.”	Intermittent tone	Alarm status	Compressor OFF
Defrost sensor abnormality	The input voltage corresponds to -50 °C or less disconnection of sensor	<Top screen> “E10:Def.sensor is opened.”	Intermittent tone	Alarm status	Heater OFF
	The input voltage corresponds to 70 °C or more short of sensor	<Top screen> “E11:Def.sensor is shorted.”	Intermittent tone	Alarm status	Heater OFF
Time to replace the fan motor for compressor	The running time is over 42,000 hours	<Top screen> “Warning:Replace comp. cooling fan motor”	---	—	---
Door alarm	Door is open for 2 minutes.	<Top screen> “Door:Open”	Intermittent tone with delay	—	Heaters, fan motor OFF
Power failure alarm	At power failure. If the power supply cord is unplugged or the power switch is turned off.	----	---	Alarm status	---

ALARMS AND SAFETY FUNCTIONS

The auto-set temperature alarm function is fitted in the temperature controller. The alarm is activated automatically when the chamber temperature deviates ± 2.5 °C (± 1.0 °C~ ± 5.0 °C) from the set temperature.

This temperature alarm function is set automatically even if under the program operation. The alarm is activated as follows under program operation.

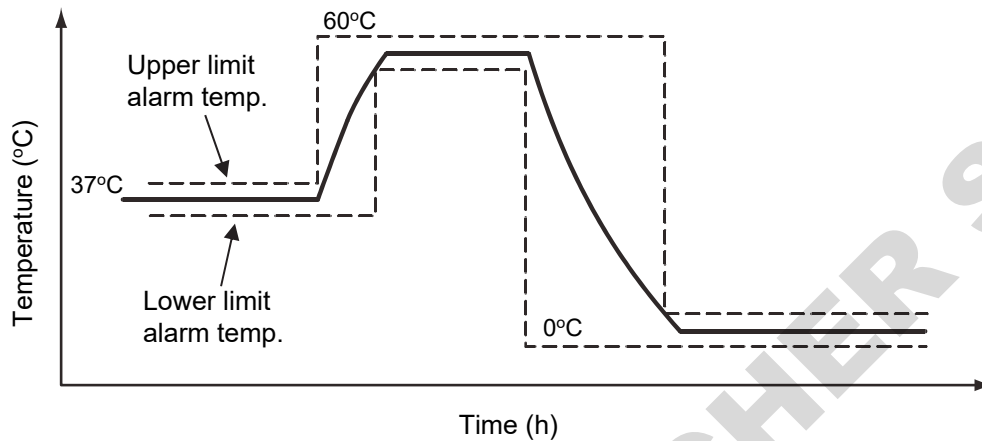

*The buzzer is stopped by pressing the alarm buzzer stop key (BUZZER), but the remote alarm keeps alarm status. The buzzer resulting from upper limit alarm and lower limit alarm cannot be silenced by the alarm buzzer stop key (BUZZER).

*The alarm may be activated when the setting of auto-set temperature alarm is small range.

MAINTENANCE

WARNING

Always disconnect the power supply to the unit prior to any repair or maintenance of the unit in order to prevent electric shock or injury.

Ensure you do not inhale or consume medication or aerosols from around the unit at the time of maintenance. These may be harmful to your health.

Cleaning

- Clean the unit once a month. Regular cleaning keeps the unit looking new.
- Use a dry cloth to wipe off small amounts of dirt on the outside and inside of the unit and all accessories. If some of them are dirty, use a cloth containing diluted neutral dishwashing detergent (Undiluted detergent may break the plastic parts. For the dilution, follow the instruction enclosed with the detergent). When a diluted neutral dishwashing detergent is used, wipe the cabinet or accessories thoroughly with a cloth soaked in clean water. Then wipe the cabinet or accessories unit with a dry cloth to eliminate the moisture.
- Never pour water onto or into the unit. Doing so can damage the electrical insulation and may cause electric shock or short circuit.
- The compressor and other mechanical part are completely sealed. This unit requires absolutely no lubrication.
- Wipe off the condensation on the outside frame or glass with a soft dry cloth.

CAUTION

Do not use brushes, acids, thinners, powdered soap or hot water for cleaning the incubator. Polishing powders or hot water can deteriorate the painted surfaces or cause deformation, discoloration or degeneration of plastic or rubber components. Be especially careful not to wipe plastic or rubber parts with volatile solvents such as benzene.

MAINTENANCE

Cleaning of evaporating tray

The evaporating tray is located at lower side on the front. Cleaning the evaporating tray twice or three times per year is recommended.

Consult our sales representative or agent when cleaning the evaporating tray.

DOMINIQUE DUTSCHER SAS

TROUBLESHOOTING

If the unit malfunctions, check out the following before calling for service. In the case of no refrigeration or poor refrigeration, transfer the stored items to another incubator before checking out.

Malfunction	Check/Remedy
When the buzzer sounds continuously	<p>In the event of lower limit temperature alarm</p> <ul style="list-style-type: none"> ▪ The set temperature of the chamber is lower than the lower limit temperature. <p>The lower limit temperature should be lower than the set temperature by more than 5 °C.</p> <p>Set the lower limit temperature after actual temperature of chamber reaches to the set temperature of operation.</p> <p>In the event of upper limit temperature alarm</p> <ul style="list-style-type: none"> ▪ The set temperature of the chamber is higher than the upper limit temperature. <p>The upper limit temperature should be higher than the set temperature by more than 5 °C.</p> <p>Set the upper limit temperature after actual temperature of chamber reaches to the set temperature of operation.</p> <ul style="list-style-type: none"> ▪ The excessive heat source is in the chamber. <p>Remove the excessive heat source.</p>
When the program operation does not function well	<p>The chamber temperature does not change according to the program.</p> <ul style="list-style-type: none"> ▪ The incubator performance (pull-up, pull-down) is not sufficient for the program setting. ▪ The over-heat or over-cool alarm temperature is wrong. <p>These temperatures should be set 5 °C higher and lower than the upper and lower limits of the temperature controller respectively. Once excessively high/low temperature limits have been determined, the operation temperatures cannot be changed significantly due to the existence of the limits for extremes of temperature. For this reason, the excessively high/low temperature limits should be set at a wide range when the program operation is set.</p>

Note:

If the malfunction is not eliminated after checking the above items, or the malfunction is not shown in the above table, contact our sales representative or agent.

DISPOSAL OF UNIT

WARNING

- If the unit is to be stored unused in an unsupervised area for an extended period, **ensure that children do not have access and doors cannot be closed completely.**
- **The disposal of the unit should be accomplished by appropriate personnel. Always remove doors** to prevent accidents such as suffocation.
- **The unit contains flammable refrigerant and flammable blowing gas. When the unit is disassembled or disposed of, the work must be performed in a well-ventilated place and avoid the place near fire.** It may cause explosions and/or a fire in case of refrigerant or gas leakage.



This label is a recycle mark complying with the Taiwanese battery regulation.

Refrigerant (applicable to MIR-554-PE)

REGULATION (EU) 2024/573 on Certain Fluorinated Greenhouse Gases

This product contains fluorinated greenhouse gases as refrigerant.

Refrigerant	GWP	Refrigerant (net) (kg)	Weight of CO2 equivalent (tonne)
R-1234yf	0.501	0.24	0.00012

Disposal of Old Equipment and Batteries**Only for European Union and countries with recycling systems**

These symbols on the products, packaging, and/or accompanying documents mean that used electrical and electronic products and batteries must not be mixed with general household waste.

For proper treatment, recovery and recycling of old products and used batteries, please take them to applicable collection points in accordance with your national legislation.

By disposing of them correctly, you will help to save valuable resources and prevent any potential negative effects on human health and the environment.

For more information about collection and recycling, please contact your local municipality.

Penalties may be applicable for incorrect disposal of this waste, in accordance with national legislation.

Note for the battery symbol (bottom symbol):

This symbol might be used in combination with a chemical symbol. In this case it complies with the requirement set by the Directive for the chemical involved.

**Likvidácia opotrebovaných zariadení a batérií****Len pre Európsku úniu a krajiny so systémom recyklácie**

Tieto symboly uvádzané na výrobkoch, balení a/alebo v sprievodnej dokumentácii informujú o tom, že opotrebované elektrické a elektronické výrobky a batérie sa nesmú likvidovať ako bežný domový odpad.

V záujme zabezpečenia správneho spôsobu likvidácie, spracovania a recyklácie odovzdajte opotrebované výrobky a batérie na špecializovanom zbernom mieste v súlade s platnou legislatívou.

Správnym spôsobom likvidácie týchto výrobkov a batérií prispějete k zachovaniu cenných zdrojov a predídete prípadným negatívnym dopadom na ľudské zdravie a životné prostredie.

Podrobnejšie informácie o zbere a recyklácii vám poskytnú miestne úrady.

Pri nesprávnej likvidácii tohto druhu odpadu môžu byť v súlade s platnou legislatívou udelené pokuty.

Poznámka týkajúca sa symbolu batérie (spodný symbol):

Tento symbol môže byť použitý spolu so symbolom chemickej značky. V takom prípade vyhovuje požiadavke stanovenej Smernicou týkajúcou sa príslušnej chemikálie.

**Изхвърляне на излезли от употреба електрически и електронни уреди и батерии****Само за Европейския съюз и страните със системи за рециклиране**

Този символ върху продуктите, опаковката и/или придружаващите документи означава, че изразходваните електрически и електронни продукти и батерии не бива да се изхвърлят в общите битови отпадъци.

Моля, предавайте старите продукти и изхабените батерии за обработка, преработка и рециклиране на компетентните пунктове за събиране на отпадъци съгласно законовите разпоредби.

Като изхвърляте тези продукти и батериите правилно, Вие помагате за запазване на ценни ресурси и за избягване на евентуално вредните влияния върху човешкото здраве и околната среда.

За повече информация относно събирането и рециклирането се обърнете към Вашето предприятие на място, предлагащо услуги във връзка с изхвърлянето на отпадъците.

Съгласно разпоредбите в страната за неправилно изхвърляне на тези отпадъци могат да бъдат наложени парични глоби.

Указание за символа батерия (символ долу):

Този символ може да е изобразен в комбинация с химически символ. В този случай това се прави поради изискванията на директивите, издадени за съответния химикал.

**Tájékoztató felhasználók számára az elhasználtott készülékek, szárazelemek és akkumulátorok begyűjtéséről és ártalmatlanításáról.****Csak az Európai Unió és olyan országok részére, amelyek begyűjtő rendszerekkel rendelkeznek**

A termékeken, a csomagoláson és/vagy a kísérő dokumentumokon szereplő szimbólumok azt jelentik, hogy az elhasználtott elektromos és elektronikus termékeket, szárazelemeket és akkumulátorokat tilos az általános háztartási hulladékkal keverni.

Az elhasználtott készülékek, szárazelemek és akkumulátorok megfelelő kezelése, hasznosítása és újrafelhasználása céljából, kérjük, hogy a helyi törvényeknek megfelelően juttassa el azokat a kijelölt gyűjtőhelyekre.

E termékek, szárazelemek és akkumulátorok előírászerű ártalmatlanításával Ön hozzájárul az értékes erőforrások megővéséhez, és megakadályozza az emberi egészség és a környezet károsodását.

Amennyiben a begyűjtéssel és újrafelhasználással kapcsolatban további kérdése lenne, kérjük, érdeklődjön a helyi önkormányzatnál.

E hulladékok szabálytalan elhelyezését a nemzeti jogszabályok büntethetik.

Megjegyzés a szárazelem- és akkumulátor-szimbólummal kapcsolatban (alsó szimbólumpélda):

Ezek a szimbólumok kémiai szimbólummal együtt alkalmazhatók. Ebben az esetben teljesíti az EU irányelvnek vegyi anyagra vonatkozó követelményét.

**Pozbywanie się zużytych urządzeń elektrycznych i elektronicznych oraz baterii.****Dotyczy wyłącznie obszaru Unii Europejskiej oraz krajów posiadających systemy zbiórki i recyklingu.**

Niniejsze symbole umieszczone na produktach, opakowaniach i/lub w dokumentacji towarzyszącej oznaczają, że nie wolno mieszać zużytych urządzeń elektrycznych i elektronicznych oraz baterii z innymi odpadami domowymi/komunalnymi.

W celu zapewnienia właściwego przetworzenia, utylizacji oraz recyklingu zużytych urządzeń elektrycznych i elektronicznych oraz zużytych baterii, należy oddawać je do wyznaczonych punktów gromadzenia odpadów zgodnie z przepisami prawa krajowego.

Poprzez prawidłowe pozbywanie się zużytych urządzeń elektrycznych i elektronicznych oraz zużytych baterii pomagasz oszczędzać cenne zasoby naturalne oraz zapobiegać potencjalnemu negatywnemu wpływowi na zdrowie człowieka oraz na stan środowiska naturalnego.

W celu uzyskania informacji o zbiórce oraz recyklingu zużytych urządzeń elektrycznych i elektronicznych oraz baterii prosimy o kontakt z władzami lokalnymi.

Za niewłaściwe pozbywanie się tych odpadów mogą grozić kary przewidziane przepisami prawa krajowego.

Dotyczy symbolu baterii (symbol poniżej):

Ten symbol może występować wraz z symbolem pierwiastka chemicznego. W takim przypadku wymagania Dyrektywy w sprawie określonego środka chemicznego są spełnione.

**Pomembna informacija za pravilno odstranjevanje izrabljene opreme in baterij****Samo za države EU in države, kjer imajo vzpostavljene sistem recikliranja odpadnih snovi**

Simboli na samem izdelku, embalaži ali spremljajočih dokumentih pomenijo, da po koncu življenske dobe aparata, z njim ni dovoljeno ravnati kot z drugimi gospodinjskimi odpadki.

Vaša dolžnost je, da izrabljeno opremo ali napravo ter baterijske vložke predate v odstranjevanje na posebna zbirna mesta za ločeno zbiranje odpadkov v okviru vaše lokalne skupnosti oziroma zastopniku, ki opravlja dejavnost prevzemanja odpadne električne in elektronske opreme.

S tem, ko jih pravilno odstranite (recikliranje in sortiranje nevarnih odpadkov) varujete naše življensko okolje ter preprečujete negativni vpliv na naravo okrog nas, na naše življensko pomembne vire in vode.

Za dodatne informacije o zbiranju in recikliranju, prosim kontaktirajte vašo lokalno skupnost.







Nepravilno odstranjevanje nevarnih in izrabljenih snovi ter naprav je lahko kaznivo dejanje.















Obvestilo za baterijski simbol (spodnji simbol):

Ta simbol se uporablja v kombinaciji s kemičnim simbolom. V takšnem primeru odgovarja zahtevi, ki jo določa direktiva za dotično kemikalijo.









DISPOSAL OF UNIT

<p>Likvidace použitých zařízení a baterií Jen pro státy Evropské unie a země s fungujícím systémem recyklace a zpracování odpadu.</p>  <p>Tyto symboly na výrobcích, jejich obalech a v doprovodné dokumentaci upozorňují na to, že se použité elektrické a elektronické zařízení, včetně baterií, nesmějí likvidovat jako běžný komunální odpad.</p> <p>Aby byla zajištěna správná likvidace a recyklace použitých výrobků a baterií, odevzdávejte je v souladu s národní legislativou na příslušných sběrných místech.</p>  <p>Správnou likvidací přispějete k úspoře cenných přírodních zdrojů a předejdete možným negativním dopadům na lidské zdraví a životní prostředí.</p> <p>O další podrobnosti o sběru a recyklaci odpadu požádejte místní úřady.</p> <p>Při nesprávné likvidaci tohoto druhu odpadu se vystavujete postihu podle národní legislativy.</p> <p>Poznámka k symbolu baterie (značka pod symbolem): Tento symbol může být použitý v kombinaci s chemickou značkou. Takový případ je souladu s požadavky směrnice pro chemické látky.</p>	<p>Vanhojen laitteiden ja paristojen hävittäminen Vain EU-jäsenmaille ja kierrätysjärjestelmää käyttäville maille</p>  <p>Tämä symboli tuotteissa, pakkauksessa ja/tai asiakirjoissa tarkoittaa, että käytettyjä sähköllä toimivia ja elektronisia tuotteita ei saa laittaa yleisiin talousjätteisiin.</p> <p>Johda vanhat tuotteet ja käytetyt paristot käsittelyä, uusiointia tai kierrätystä varten vastaaviin keräyspisteisiin laissa annettujen määräysten mukaisesti.</p> <p>Hävittämällä tuotteet asiaankuuluvasti, autat samalla suojaamaan arvokkaita luonnonvaroja ja estämään mahdollisia negatiivisia vaikutuksia ihmiseen ja luontoon.</p> <p>Lisätietoa keräämisestä ja kierrätyksestä saa paikalliselta jätehuollosta vastuulliselta viranomaiselta.</p> <p>Maiden lainsäädännön mukaisesti tämän jätteen määräystenvastaisesta hävittämisestä voidaan antaa sakkorangaistuksia.</p> <p>Huomautus paristosymbolista (symboli alhaalla): Tämä symboli voidaan näyttää jonkin kemiallisen symbolin yhteydessä. Siinä tapauksessa se perustuu vastaaviin direktiiveihin, jotka on annettu kyseessä olevalle kemikaalille.</p> 
<p>Eski Ekipman ve Bataryaların Tasfiyesi Sadece Avrupa Birliği ve geri dönüşüm sistemleri olan ülkeler için</p>  <p>Ürünlerin, ambalajın ve/veya ek olarak gelen belgelerin üzerinde bu semboller, elektrikli ve elektronik ürünlerin ve bataryaların genel ev atıklarıyla karıştırılmaması gerektiği anlamına gelir.</p> <p>Eski ürünlerin ve kullanılmış bataryaların doğru şekilde işlenmesi, geri kazanımı ve geri dönüşümü için lütfen bunları ulusal kanunlara uygun olan toplama noktalarına götürün.</p> <p>Bunları doğru şekilde tasfiye ederek değerli kaynakları kurtarmaya ve insan sağlığı ve çevre üzerinde olabilecek olumsuz etkileri önlemeye yardım edeceksiniz.</p> <p>Toplama ve geri dönüşüm hakkında daha fazla bilgi için lütfen bölgenizdeki belediye ile irtibat kurun.</p> <p>Bu atığın yanlış şekilde tasfiye edilmesi durumunda ulusal kanunlar uyarınca cezalar verilebilir.</p> <p>Batarya sembolüne bakın (alttaki sembol): Bu sembol bir kimyasal sembolü ile birlikte kullanılmıř olabilir. Bu durumda batarya, kullanılan kimyasal maddeye yönelik Direktif ile belirlenen şartı karşıllıyordur.</p> 	<p>Entsorgung von Altgeräten und Batterien Nur für die Europäische Union und Länder mit Recyclingsystemen</p>  <p>Dieses Symbol, auf den Produkten, der Verpackung und/oder den Begleitdokumenten, bedeutet, dass gebrauchte elektrische und elektronische Produkte sowie Batterien nicht in den allgemeinen Hausmüll gegeben werden dürfen.</p> <p>Bitte führen Sie alte Produkte und verbrauchte Batterien zur Behandlung, Aufarbeitung bzw. zum Recycling gemäß den gesetzlichen Bestimmungen den zuständigen Sammelpunkten zu. Endnutzer sind in Deutschland gesetzlich zur Rückgabe von Altbatterien an einer geeigneten Annahmestelle verpflichtet. Batterien können im Handelsgeschäft unentgeltlich zurückgegeben werden.</p> <p>Indem Sie diese Produkte und Batterien ordnungsgemäß entsorgen, helfen Sie dabei, wertvolle Ressourcen zu schützen und eventuelle negative Auswirkungen auf die menschliche Gesundheit und die Umwelt zu vermeiden.</p> <p>Für mehr Informationen zu Sammlung und Recycling, wenden Sie sich bitte an Ihren örtlichen Abfallentsorgungsdienstleister.</p> <p>Gemäß Landesvorschriften können wegen nicht ordnungsgemäßer Entsorgung dieses Abfalls Strafgeľder verhängt werden.</p> <p>Hinweis für das Batteriesymbol (Symbol unten): Dieses Symbol kann in Kombination mit einem chemischen Symbol abgebildet sein. In diesem Fall erfolgt dieses auf Grund der Anforderungen derjenigen Richtlinien, die für die betreffende Chemikalie erlassen wurden.</p> 
<p>L'élimination des équipements et des batteries usagés Applicable uniquement dans les pays membres de l'Union européenne et les pays disposant de systèmes de recyclage.</p>  <p>Apposé sur le produit lui-même, sur son emballage, ou figurant dans la documentation qui l'accompagne, ce pictogramme indique que les piles, appareils électriques et électroniques usagés, doivent être séparées des ordures ménagères.</p> <p>Afin de permettre le traitement, la valorisation et le recyclage adéquats des piles et des appareils usagés, veuillez les porter à l'un des points de collecte prévus, conformément à la législation nationale en vigueur.</p> <p>En les éliminant conformément à la réglementation en vigueur, vous contribuez à éviter le gaspillage de ressources précieuses ainsi qu'à protéger la santé humaine et l'environnement.</p> <p>Pour de plus amples renseignements sur la collecte et le recyclage, veuillez vous renseigner auprès des collectivités locales.</p> <p>Le non-respect de la réglementation relative à l'élimination des déchets est passible d'une peine d'amende.</p> <p>Note relative au pictogramme à apposer sur les piles (pictogramme du bas) : Si ce pictogramme est combiné avec un symbole chimique, il répond également aux exigences posées par la Directive relative au produit chimique concerné.</p> 	<p>Eliminación de Aparatos Viejos y de Pilas y Baterías Solamente para la Unión Europea y países con sistemas de reciclado.</p>  <p>Estos símbolos en los productos, su embalaje o en los documentos que los acompañan significan que los productos eléctricos y electrónicos y pilas y baterías usadas no deben mezclarse con los residuos domésticos.</p> <p>Para el adecuado tratamiento, recuperación y reciclaje de los productos viejos y pilas y baterías usadas llévelos a los puntos de recogida de acuerdo con su legislación nacional. En España, los usuarios están obligados a entregar las pilas en los correspondientes puntos de recogida. En cualquier caso, la entrega por los usuarios será sin coste alguno para éstos. El coste de la gestión medioambiental de los residuos de pilas, acumuladores y baterías está incluido en el precio de venta.</p> <p>Si los elimina correctamente ayudará a preservar valiosos recursos y evitará potenciales efectos negativos sobre la salud de las personas y sobre el medio ambiente.</p> <p>Para más información sobre la recogida u reciclaje, por favor contacte con su ayuntamiento.</p> <p>Puede haber sanciones por una incorrecta eliminación de este residuo, de acuerdo con la legislación nacional.</p> <p>Nota para el símbolo de pilas y baterías (símbolo debajo): Este símbolo puede usarse en combinación con el símbolo químico. En este caso, cumple con los requisitos de la Directiva del producto químico indicado.</p> 

<p>Smaltimento di vecchie apparecchiature e batterie usate Solo per Unione Europea e Nazioni con sistemi di raccolta e smaltimento</p>   <p>Questi simboli sui prodotti, sull'imballaggio e/o sulle documentazioni o manuali accompagnanti i prodotti indicano che i prodotti elettrici, elettronici e le batterie usate non devono essere buttati nei rifiuti domestici generici.</p> <p>Per un trattamento adeguato, recupero e riciclaggio di vecchi prodotti e batterie usate vi invitiamo a portarli negli appositi punti di raccolta secondo la legislazione vigente nel vostro paese.</p> <p>Con uno smaltimento corretto, contribuirete a salvare importanti risorse e ad evitare i potenziali effetti negativi sulla salute umana e sull'ambiente.</p> <p>Per ulteriori informazioni su raccolta e riciclaggio, vi invitiamo a contattare il vostro comune.</p> <p>Lo smaltimento non corretto di questi rifiuti potrebbe comportare sanzioni in accordo con la legislazione nazionale.</p> <p>Note per il simbolo batterie (simbolo sotto): Questo simbolo può essere usato in combinazione con un simbolo chimico. In questo caso è conforme ai requisiti indicati dalla Direttiva per il prodotto chimico in questione.</p>	<p>Eliminação de Equipamentos Usados e Baterias Apenas para a União Europeia e países com sistemas de reciclagem</p>   <p>Estes símbolos nos produtos, embalagens, e/ou documentos que os acompanham indicam que os produtos elétricos e eletrônicos e as baterias usados não podem ser misturados com os resíduos urbanos indiferenciados.</p> <p>Para um tratamento adequado, reutilização e reciclagem de produtos e baterias usados, solicitamos que os coloque em pontos de recolha próprios, em conformidade com a respetiva legislação nacional.</p> <p>Ao eliminar estes produtos corretamente estará a ajudar a poupar recursos valiosos e a prevenir quaisquer potenciais efeitos negativos sobre o ambiente e a saúde humana.</p> <p>Para mais informações acerca da recolha e reciclagem, por favor contacte a sua autarquia local.</p> <p>De acordo com a legislação nacional podem ser aplicadas contraordenações pela eliminação incorreta destes resíduos.</p> <p>Nota para o símbolo da bateria (símbolo na parte inferior): Este símbolo pode ser utilizado conjuntamente com um símbolo químico. Neste caso estará em conformidade com o estabelecido na Diretiva referente aos produtos químicos em causa.</p>
<p>Depunerea la deșeuri a echipamentelor și a bateriilor vechi Doar pentru Uniunea Europeană și pentru țările cu sisteme de reciclare</p>   <p>Aceste simboluri de pe produse, ambalaje și/sau documentele însoțitoare indică faptul că produsele electrice și electronice, precum și bateriile uzate nu trebuie să fie amestecate cu deșeurile menajere obișnuite.</p> <p>Pentru un tratament corespunzător, pentru recuperarea și reciclarea produselor vechi și a bateriilor uzate, vă rugăm să le depuneți la punctele de colectare special amenajate, în conformitate cu legislația națională.</p> <p>Prin depunerea corespunzătoare a acestora la deșeuri, veți ajuta la economisirea unor resurse valoroase și veți preveni potențiale efecte negative asupra sănătății umane și asupra mediului înconjurător.</p> <p>Pentru mai multe informații despre colectare și reciclare, vă rugăm să contactați autoritățile locale.</p> <p>Este posibil ca depunerea încorectă la deșeuri să fie pedepsită în conformitate cu legile naționale.</p> <p>Notă pentru simbolul de baterie (ultimele două exemple de simboluri): Acest simbol poate fi utilizat în combinație cu un simbol chimic. În acest caz, acesta este conform cu cerințele stabilite de Directivă pentru elementul chimic în cauză.</p>	<p>Indsamling af elektroniskrot og brugte batterier Kun for Den Europæiske Union og lande med retursystemer</p>   <p>Disse symboler på produkter, emballage og/eller ledsagedokumenter betyder, at brugte elektriske og elektroniske produkter og batterier ikke må blandes med almindeligt husholdningsaffald.</p> <p>For korrekt behandling, indsamling og genbrug af gamle produkter og batterier, skal du tage dem til indsamlingssteder i overensstemmelse med den nationale lovgivning.</p> <p>Ved at skaffe sig af med dem på korrekt vis hjælper du med til at spare værdifulde ressourcer og forhindre eventuelle negative påvirkninger af menneskers sundhed og miljøet.</p> <p>Ønsker du mere udførlig information om indsamling og genbrug skal du kontakte din kommune.</p> <p>Usagkyndig bortskaffelse af elektroniskrot og batterier kan eventuelt udløse bødeforlæggelse.</p> <p>Information om batterisymbol (eksempler nedenfor): Dette symbol kan anvendes sammen med et kemisk symbol. I så fald opfylder det kravene for det direktiv, som er blevet fastlagt for det pågældende kemikalie.</p>
<p>Senų prietaisų ir akumuliatorių utilizavimas Taikoma tik Europos Sąjungai ir šalims, kuriose naudojamas perdirbimo sistemos</p>   <p>Jeigu ant pakuotės ir (arba) lydimojuose dokumentuose nurodytas šis simbolis, vadinasi, naudotų elektrinių ir elektroninių gaminių ir akumuliatorių negalima išmesti kartu įprastomis buitiniemis atliekomis.</p> <p>Senus produktus ir naudotus akumuliatorius perduokite apdirbti, likviduoti arba perdirbti kompetentingiems surinkimo punktais pagal įstatymų galios potvarkius.</p> <p>Šiuos gaminius ir akumuliatorius perdavę tinkamai utilizuoti, padėsite išsaugoti vertingus išteklius ir išvengti neigiamo poveikio žmogaus sveikatai ir aplinkai.</p> <p>Jeigu norite gauti daugiau informacijos apie surinkimą ir perdirbimą, kreipkitės į vietos atliekų utilizavimo paslaugų teikėją.</p> <p>Remiantis šalyje galiojančiais potvarkiais, už netinkamą tokių atliekų utilizavimą gali būti skirta bauda.</p> <p>Akumuliatoriaus simbolio nuoroda (simbolis apačioje): Kartu su šiuo simboliu gali būti pateiktas cheminių medžiagų simbolis. Šis simbolis pateikiamas, kai būtina laikytis atitinkamiems chemikalams taikomų direktyvų reikalavimų.</p>	<p>Rimi ta' Tagħmir Antik u Batteriji Għall-Unjoni Ewropea u għall-pajjiżi b'sistemi ta' riċiklaġġ biss</p>   <p>Dawn is-simboli fuq il-prodotti, l-imballaġġ u/jew id-dokumenti ta' akkumpanjament ifissru li prodotti elettrici u elettronici u batteriji uzati ma jridux jigu mhallta ma' skart domestiku generali.</p> <p>Għal trattament, irkupru u riċiklaġġ xieraq ta' prodotti antik u batteriji uzati, jekk jogħġbok huqdom f'punti tal-ġbir applikabbli f'konformità mal-leġiżlazzjoni nazzjonali tiegħek.</p> <p>Billi tarmihom b'mod xieraq, tgħin sabiex tikkonserva riżorsi prezzjużi u tipprevjeni kwalunkwe effett negattiv potenzjali fuq is-saħħa tal-bniedem u l-ambjent.</p> <p>Għal aktar informazzjoni dwar il-ġbir u r-riċiklaġġ, jekk jogħġbok ikkuntattja l-il-municipalitá lokali tiegħek.</p> <p>F'każ ta' rimi mhux korrett ta' dan l-iskart jistgħu japplikaw penali, f'konformità mal-leġiżlazzjoni nazzjonali.</p> <p>Nota għas-simbolu tal-batterija (simbolu ta' taħt): Dan is-simbolu jista' jintuża f'kombinazzjoni ma' simbolu tal-kimika. F'dan il-każ jikkonforma mar-rekwiżit stabbilit mid-Direttiva għall-kimika involuta.</p>
<p>Zbrinjavanje starih uređaja i baterija Samo za Europsku uniju i zemlje koje posjeduju sustav recikliranja</p>   <p>Ovaj simbol na proizvodima, pakiranju i/ili popratnim dokumentima znači da se iskorišteni električni i elektronički proizvodi te baterije ne smiju bacati u kućanski otpad.</p> <p>Molimo vas da prema zakonskim odredbama stare proizvode i istrošene baterije predate na ovlaštenim sabiralištima na daljnju obradu, pripremu odn. recikliranje.</p> <p>Ako te proizvode i baterije propisno zbrinete, pomažete pri zaštiti dragocjenih resursa, a istovremeno i izbjegavate eventualne negativne utjecaje na ljudsko zdravlje i okoliš.</p> <p>Za više informacija o zbrinjavanju i recikliranju obratite se svojem lokalnom komunalnom poduzeću.</p> <p>Zbog nepropisnog zbrinjavanja ovog otpada mogu se, ovisno o lokalnim propisima zemlje, izreći i novčane kazne.</p> <p>Napomena za simbol baterije : Ovaj simbol može biti prikazan samo u kombinaciji s kemijskim simbolom. U tom se slučaju upotrebljava na temelju zahtjeva onih direktiva koje su donesene za dotičnu kemikaliju.</p>	

DISPOSAL OF UNIT

<p>Avfallshandtering av produkter och batterier Endast för Europeiska Unionen och länder med återvinningssystem</p>  <p>Dessa symboler på produkter, förpackningar och/eller medföljande dokument betyder att förbrukade elektriska och elektroniska produkter och batterier inte får blandas med vanliga hushållsoppor.</p> <p>För att gamla produkter och använda batterier ska hanteras och återvinnas på rätt sätt ska dom lämnas till passande uppsamlingsställe i enlighet med nationella bestämmelser.</p> <p>Genom att ta göra det korrekt hjälper du till att spara värdefulla resurser och förhindrar eventuella negativa effekter på människors hälsa och på miljön.</p> <p>För mer information om insamling och återvinning kontakta din kommun.</p> <p>Olämplig avfallshandtering kan beläggas med böter i enlighet med nationella bestämmelser.</p> <p>Notering till batterisymbolen (nedanför): Denna symbol kan användas i kombination med en kemisk symbol. I detta fall uppfyller den de krav som ställs i direktivet för den aktuella kemikalien.</p>	<p>Brukerinformasjon om innsamling av gammelt utstyr og brukte batterier Bare for EU og land med retursystemer</p>  <p>Slike symboler på produkter, emballasje, og/eller på medfølgende dokumenter betyr at brukte elektriske/elektroniske produkter og batterier ikke må blandes med vanlig husholdningsavfall.</p> <p>For riktig håndtering og gjenvinning av gamle produkter og brukte batterier, vennligst lever dem til innsamlingssteder i samsvar med nasjonallovgivning.</p> <p>Ved riktig håndtering av disse produktene og batteriene, hjelper du til med å spare verdifulle ressurser og forhindre potensielle negative effekter på menneskers helse og miljø.</p> <p>Før mer informasjon om innsamling og gjenvinning vennligst ta kontakt med din kommune.</p> <p>Ukorrekt håndtering av dette avfallet kan medføre straffansvar, i overensstemmelse med nasjonal lovgivning.</p> <p>Merknader for batterisymbolen (nederste symbol): Dette symbolet kan bli brukt i kombinasjon med et kjemisk symbol. I dette tilfellet etterkommer det kravet satt av direktivet for det kjemikallet det gjelder.</p>
<p>Het ontdoen van oude apparatuur en batterijen. Enkel voor de Europese Unie en landen met recycle systemen.</p>  <p>Deze symbolen op de producten, verpakkingen en/of begeleidende documenten betekenen dat gebruikte elektrische en elektronische producten en batterijen niet samen mogen worden weggegooid met de rest van het huishoudelijk afval.</p> <p>Voor een juiste verwerking, hergebruik en recycling van oude producten en batterijen, gelieve deze in te leveren bij de desbetreffende inleverpunten in overeenstemming met uw nationale wetgeving.</p> <p>Door ze op de juiste wijze weg te gooien, helpt u mee met het besparen van kostbare hulpbronnen en voorkomt u potentiële negatieve effecten op de volksgezondheid en het milieu.</p> <p>Voor meer informatie over inzameling en recycling kunt u contact opnemen met uw plaatselijke gemeente.</p> <p>Afhankelijk van uw nationale wetgeving kunnen er boetes worden opgelegd bij het onjuist weggooiden van dit soort afval.</p> <p>Let op: het batterij symbool (Onderstaand symbool). Dit symbool kan in combinatie met een chemisch symbool gebruikt worden. In dit geval volstaan de eisen, die zijn vastgesteld in de richtlijnen van de desbetreffende chemische stof.</p>	<p>Απόρριψη παλαιών συσκευών και μπαταριών Μόνο για την Ευρωπαϊκή Ένωση και χώρες με συστήματα ανακύκλωσης</p>  <p>Το σύμβολο αυτό, πάνω στα προϊόντα, τη συσκευασία ή/και τα συνοδευτικά έγγραφα, υποδηλώνει ότι τα χρησιμοποιημένα ηλεκτρικά και ηλεκτρονικά προϊόντα, καθώς και οι μπαταρίες, δεν πρέπει να απορριπτούν στα κοινά οικιακά απορρίμματα.</p> <p>Παρακαλούμε παραδώστε τα παλαιά προϊόντα και τις χρησιμοποιημένες μπαταρίες για διαχείριση, επεξεργασία ή/και ανακύκλωση σύμφωνα με τις νομικές διατάξεις των αρμόδιων αρχών αποκομιδής.</p> <p>Με την ορθή απόρριψη αυτών των προϊόντων και μπαταριών, συμβάλλετε στην εξοικονόμηση πολύτιμων πόρων και την αποφυγή τυχόν αρνητικών επιπτώσεων στην ανθρώπινη υγεία και το περιβάλλον.</p> <p>Για περισσότερες πληροφορίες σχετικά με τη συλλογή και την ανακύκλωση, παρακαλούμε απευθυνθείτε στις κατά τόπους υπηρεσίες συγκομιδής απορριμμάτων.</p> <p>Σε περίπτωση αντικανονικής απόρριψης αυτού του προϊόντος ενδεχομένως να επιβληθούν πρόστιμα, ανάλογα με τη νομοθεσία του εκάστοτε κράτους.</p> <p>Σημείωση για το σύμβολο μπαταρίας (σύμβολο κάτω): Το σύμβολο αυτό μπορεί να απεικονίζεται σε συνδυασμό με ένα χημικό σύμβολο. Αυτό γίνεται ώστε να υπάρχει συμφωνία με τις απαιτήσεις των εκάστοτε οδηγιών, που εκδόθηκαν για το εν λόγω χημικό.</p>
<p>Nolietoto elektronisko ierīču un elektroprēču un bateriju utilizācija Tikai Eiropas valstīs ar utilizācijas sistēmu</p>  <p>Šis simbols, kas izvietots uz ražojumiem, iesaiņojuma un/vai pavaddokumentiem nozīmē, ka nolietotās elektroniskās ierīces un elektroprēces, kā arī baterijas nedrīkst izmest kopā ar parastiem mājāsaimniecības atkritumiem.</p> <p>Nogādājiet nolietotos ražojumus un nokalpojušās baterijas tālākai apstrādei, pārstrādei, resp., materiālu otrreizējai pārstrādei attiecīgajās atkritumu savākšanas vietās saskaņā spēkā esošajām likumdošanas prasībām.</p> <p>Nododot šos ražojumus un baterijas profesionālai utilizācijai, jūs palīdzēsiet saudzēt vērtīgos resursus un novērsīsiet iespējamu kaitējumu cilvēku veselībai un un apkārtnēji videi.</p> <p>Lai iegūtu plašāku informāciju par atkritumu savākšanu un otrreizējo pārstrādi, lūdzam vērsties savā vietējā atkritumu pārstrādes uzņēmumā.</p> <p>Saskaņā ar nacionālo likumdošanu par nepareizu šāda veida atkritumu utilizāciju var uzlikt naudas sodu.</p> <p>Norāde par baterijas simbolu (simbols apakšā): Šis simbols var būt attēlots kombinācijā ar ķīmiskās vielas simbolu. Tādā gadījumā tas ir apzīmēts atbilstoši attiecīgo Direktīvu prasībām, kas pieņemtas attiecībā uz attiecīgo ķīmikāliju.</p>	<p>Уклањање старих апарата и батерија Само за Европску Унију и државе са системима рециклирања</p>  <p>Овај симбол на производима, паковању и/или пратећим документима значи да коришћени електрични и електронски апарати не смеју бити бачени у обично кућно њубре.</p> <p>Молимо да сходно законским одредбама однесете старе производе и искоришћене батерије у надлежна сабирна места на третман, прераду, односно рециклирање.</p> <p>Тиме што ћете ове производе и батерије правилно уклонити помажете да се притом заштите вредни ресурси и избегну евентуална негативна дејства на људско здравље и човекову околину.</p> <p>Молимо да се за више информација у вези сакупљања и рециклирања обратите Вашој месној служби за уклањање отпада.</p> <p>За непрописно уклањање овог отпада могу бити изречене новчане казне према прописима државе.</p> <p>Упутство за симбол за батерију (симбол доле): Овај симбол може бити илустрован у комбинацији са хемијским симболом. У том случају ово следи на основу захтева оних смерница које су донешене за дотичне хемикалије.</p>
<p>Vanade seadmete ja patareide jäätmekäitlus Ainult Euroopa Liidule ja ringlussevõtu süsteemidega riikidele</p>  <p>Toodetel, pakendil ja/või kaasasolevatel dokumentidel oleval sümboolil tähendavad, et elektri- ja elektroonikatooted ja patareid ei tohi visata tavaliste olmejäätmete hulka.</p> <p>Vanade toodete ja kasutatud patareide nõuetekohaseks töötlemiseks, taastamiseks ja ringlusse võtmiseks viige need ettenähtud kogumiskohtadesse vastavalt riiklikele õigusaktidele.</p> <p>Nende toodete ja patareide korrektsesse kõrvaldamisega aitate säästa hinnalisi ressursse ning vältida võimalikke kahjulikke mõjusid inimeste tervisele ja keskkonnale.</p> <p>Täpsema teabe saamiseks kogumise ja ringlussevõtu kohta pöörduge kohaliku omavalitsuse poole.</p> <p>Vastavalt riiklikele õigusaktidele võib selliste jäätmete ebakorrektsesse käitlemisega kaasneda trahv.</p> <p>Märkus patarei sümboli kohta : Seda sümboolit võib kasutada kombinatsioonis keemilise sümboliga. Sellisel juhul vastab see asjaomase kemikaali kasutamist reguleeriva direktiivi nõuetele.</p>	

LOW HUMIDITY MODE

The humidity in the chamber goes up over 90 %R.H. if the unit is running without low humidity mode when moisturized material is put inside the chamber. This may result in the condensation on the inside of the door or clearance in the chamber.

The low humidity mode is a running mode to reduce the condensation under above condition by running control with the set temperature between 20 °C and 40 °C

Refer to page 40 for the setting of low humidity mode.

*Default setting of the low humidity mode is 0 (No).

[When selecting the low humidity mode]

The compressor is on/off more than normal to reduce the condensation in the chamber. Accordingly, the fluctuation of the chamber humidity is more than the normal running mode.

The chamber humidity varies between 80 %R.H. and 50 %R.H. when the chamber temperature is set to 37 °C and the ambient temperature is 20 °C.

CAUTION

The material in the chamber may be dried depending on the usage condition when the low humidity mode is selected. Do not select the low humidity mode when the drying of culture media should be avoided.

[When selecting the normal mode (no low humidity mode)]

Pay attention to the following when the chamber temperature setting is lower than the ambient temperature with moisturized material put inside the chamber.


- The condensation may be found on the inside of the door or clearance in the chamber. Wipe off the condensation with a dry cloth.
- The condensation is held on the dew saucer and drained into the evaporating tray. The evaporating pipe is not heated when the compressor is off. Therefore, it is needed to clean the evaporating tray once a week.

*The amount of condensation depends on the usage condition.

CAUTION

Clean the evaporating tray regularly when selecting the normal mode (no low humidity mode). Spilled water from the evaporating tray causes the mold.

*With the normal mode, the drained water may be spilled from the evaporating tray when the condensation is found on the door. In this case, take out the drain pipe from the port and drain the water to a container or bucket.

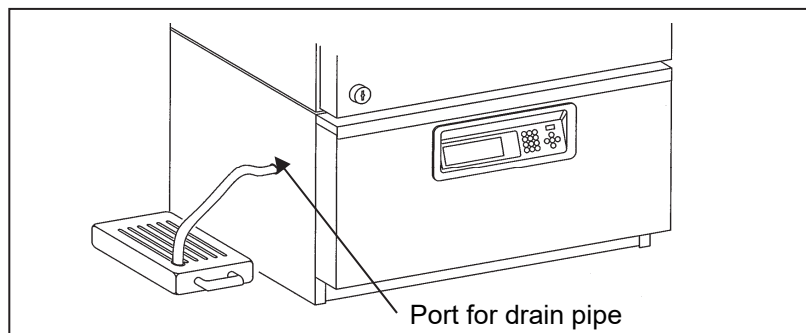


Consult our sales representative or agent when using the drain pipe.

PERFORMANCE DATA

Graph 1

Chamber temperature pull-down and pull-up characteristics

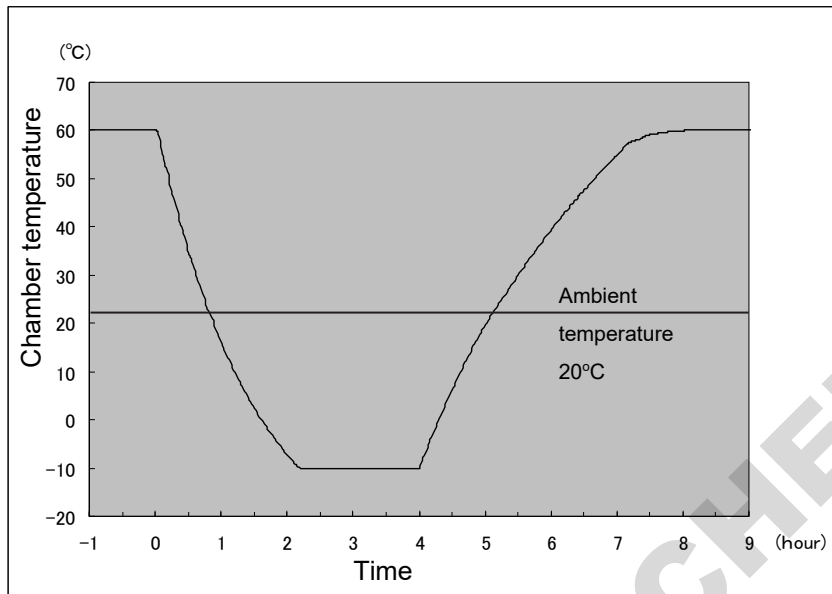

Notes:

- The performance data is the data with the lamp OFF.
- The performance may be varied slightly depending on each unit or running condition.

SPECIFICATIONS

Product name	Cooled Incubator MIR-554
External dimensions	W800 mm x D832 mm x H1810 mm W31.50 inch x D32.76 inch x H71.26 inch
Internal dimensions	W640 mm x D550 mm x H1160 mm W25.20 inch x D21.65 inch x H45.67 inch
Effective capacity	406 L (14.33 cu.ft.)
Exterior	Painted steel
Interior	Stainless steel
Door	Painted steel
Shelf	Polyethylene coated steel wire, Adjustable, 5 shelves Inner dimensions: Upper 4 W580 mm x D440 mm (W22.83 inch x D17.32 inch) Bottom 1 W580 mm x D490 mm (W22.83 inch x D19.29 inch) Max. load: 50 kg (110.23 lb)
Access port	Inner diameter 40 mm (left and right side)
Insulation	Rigid polyurethane foamed-in place
Cooling method	Forced air circulation
Compressor	Reciprocated compressor Output: 270 W
Evaporator	Fin and tube type
Condenser	Wire and tube type
Refrigerant	R-1234yf
Defrost heater	306 W/335 W/365 W (MIR-554-PE) 332 W (MIR-554-PA)
Temperature controller	Microprocessor, PID control (compressor; ON-OFF)
Temperature display	Digital display
Alarm	High temp. alarm, Low temp. alarm, Independent over-heat/over-cool limiter
Remote alarm contact	Capacity; DC 30 V, 2 A *2
Program function	12 steps, 1 to 98 repeating or unlimited, Max. 10 programs memorized
Memory backup	Nonvolatile memory
Accessories	4 rubber caps for access port, 5 shelves, 20 clips, 1 set of key
Weight	195 kg (430 lb)
Optional components	Light add-on kit (MIR-L15) *1, Inner door (MIR-55ID) Interface board (MTR-L03) *2, *3, Interface board (MTR-480) *2, *3 Analog Interface board (MTR-420MA) *2, *3

*1: This kit is specified for LED lights.

*2: It is recommended to use standard signal and interface cables with a maximum length of 30 meters.

*3: For purchase of the interface boards, contact our sales representative or agent.

Notes:

- Design or specifications are subject to change without notice.
- Refer to the updated catalogue when ordering an optional component.

PERFORMANCE

Product name	Cooled Incubator MIR-554	
Model number	MIR-554-PE	MIR-554-PA
Control range	-10 °C~+60 °C (ambient temp: +5 °C~+35 °C, no load)*1*2	
Temperature fluctuation	±1.5 °C ON-OFF control (set: 5 °C, ambient temp: 20 °C, no load) ±0.2 °C PID control (set: 50 °C, ambient temp: 20 °C, no load)	
Temperature uniformity	±0.5 °C (set: 37 °C, ambient temp.: 20 °C, no load)	
Noise level	45 dB (A scale)	
Maximum pressure	1700 kPa	
Rated voltage	AC 220 V/230 V/240 V	AC 110 V/115 V
Rated frequency	50 Hz	60 Hz
Power consumption	250 W/265 W/290 W	485 W (Max.)
Environmental conditions	Ambient temperature: +5 °C~+35 °C, Humidity: less than 80% R.H.	

*1: The control range when the optional inner door (MIR-55ID) installed is -10 °C~+50 °C.
(Ambient temp.: +5 °C~+35 °C, no load)

*2: The lighting is available only with temperature range between +2 °C and +50 °C when the optional light add on kit (MIR-L15) is installed. In the case of temperature out of range, the lighting is not usable.

Notes:

- The unit with CE mark complies with EU directives.
- Each data of this product is measured by our standard.
- All the described performances are applied for the rated supply voltage and the frequency.
- Design or specifications will be subject to change without notice.

SAFETY CHECK SHEET



CAUTION

Please copy and fill out this form before servicing.
Hand over the form to the service engineer for their
and your safety.

Safety check sheet

1. Stored material

Risk of infection: Yes No Maybe

Risk of toxicity: Yes No Maybe

Risk from radioactive sources: Yes No Maybe

List all potentially hazardous materials that have been stored in this unit:

2. Contamination in the unit

a) Contamination Yes No Maybe

Types of contamination (if any):

b) Decontaminated Yes No

Methods used for the decontamination work:

3. Status of the unit

a) The unit is now safe to work on Yes No

b) If the answer is "No,"
Details on the danger:

Measures we should take to reduce the danger:

Date:

Signature:

Address, Division:

Telephone:

Product name:
Cooled Incubator

Model No.
MIR-

Serial number:

Date of Installation:

Please decontaminate the unit yourself before calling the service engineer.

DOMINIQUE DUTSCHER SAS

PHC Corporation

1-1-1 Sakada, Oizumi-machi, Ora-gun, Gunma 370-0596, Japan

© PHC Corporation 2024



LDCL084900-3

Printed in Japan
LDCL084900-3
J0224-30825