


Use of LYPHAN Paper Strips to measure pH

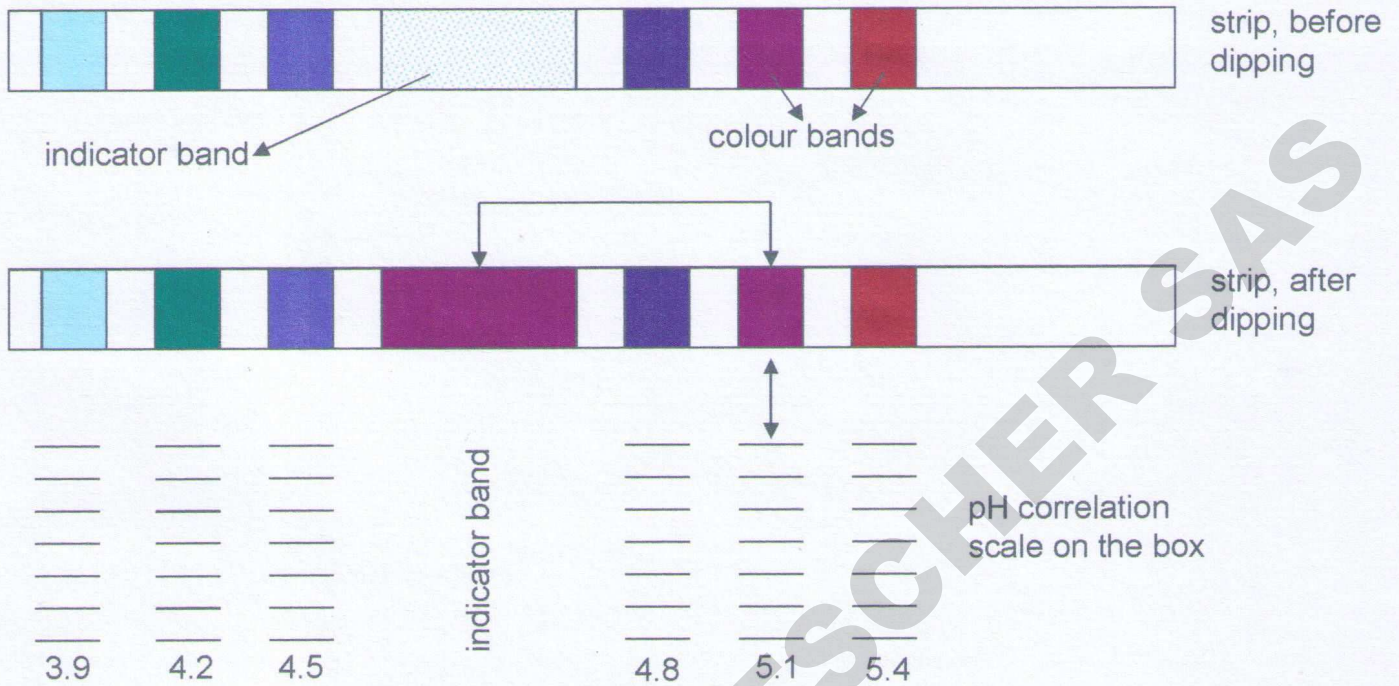

In the above example, colour of the indicator band after dipping in sample matches with that of colour band corresponding to pH value of 5.1. Therefore, the sample pH is 5.1.

IMPORTANT: For reliable results, dipping in the sample and reading of pH must be completed within a few seconds. Comparing colour against a light (i.e. in transmitted mode) provides better accuracy.