



# Sera-Xtracta

## Virus/Pathogen Kit

User guide

DOMINIQUE DUTSCHER SAS

# 1 Introduction

## Product codes

29506009 (96 extractions)  
29514201 (1000 extractions)

## Important

Read the instructions carefully before using the products.

## Intended use

The product is intended for Research Use Only and shall not be used in any clinical or *in vitro* procedures for diagnostic purposes. Do not use internally or externally in humans or animals.

## Safety

For use, handling and disposal of the product, refer to the Safety Data Sheets. Good laboratory practices should be followed at all times.

## Storage

All kit components should be stored at room temperature (15°C–30°C).  
Once reconstituted, store Proteinase K at 2°C–8°C.

## Expiry

For expiry date, refer to outer packaging label.

Reconstituted Proteinase K solution is stable for at least 4 months when stored at 2°C–8°C.

## 2 Components

### Kit components

Pack sizes:

Component	96 extraction kit (29506009)	1000 extraction kit (29514201)
Binding / Lysis Reagent	60 mL	630 mL
Wash buffer	100 mL	1000 mL
SeraSil-Mag™ 400 beads	1.1 mL	10.4 mL
SeraSil-Mag 700 beads	1.1 mL	10.4 mL
Proteinase K	30 mg	2 × 110 mg

### Materials to be supplied by the user

#### Chemicals:

- Ethanol (absolute)
- Nuclease free water

#### Equipment:

- 1.5–2.0 mL microtubes, DNase / RNase-free.
- Laboratory heating block (thermoblock), for 1.5–2.0 mL microtubes.
- Vortex Mixer
- Bench-top centrifuges for 1.5–2.0 mL microtubes.
- Magnetic separation racks, suitable for 1.5–2.0 mL microtubes.
- Pipette tips with aerosol barrier

**Note:** All tubes and pipette tips should be DNase / RNase free grade. The working environment should also be subject to cleaning procedures to minimize the presence of extraneous DNases, RNases and other DNA / RNA material originating from operators, samples and other biological sources.

### 3 Description

Cytiva has developed a kit incorporating its magnetic bead based technology (Sera-Xtracta™ Virus/Pathogen Kit), for the isolation of viral/bacterial nucleic acids (RNA and DNA). The Sera-Xtracta Virus/Pathogen Kit has been optimised for the isolation of nucleic acid from swab samples collected in universal transport media routinely used to collect, store and transport clinical samples.

Infectious diseases affect millions of people every year. Particularly virulent and multi-drug resistant agents are increasingly responsible for infections with ever-expanding complexities. Molecular diagnostic laboratories and their test developers need to design, manufacture, and validate assays for these pathogenic agents. This requires the successful purification of high-quality nucleic acid which is essential to any molecular research and testing workflow. The nucleic acid purification process can be a bottleneck because sufficient nucleic acid from biological samples is required to meet a sensitivity threshold for an assay or tests which are designed to help mapping or making informed decisions on latent and active infections.

To address this bottleneck, Cytiva has developed a robust extraction chemistry optimized with SeraSil-Mag magnetic beads for total nucleic acid (DNA/RNA) from various pathogen types. Our optimized reagent chemistry ensures total nucleic acid is selectively bound to the superparamagnetic SeraSil-Mag bead while impurities are efficiently removed during the quick wash steps. The resulting high quality total nucleic acid is then eluted from the beads. The rapid workflow (Fig1) is optimized for processing 100–400 µL of transport media to yield nucleic acid suitable for sensitive molecular testing including quantitative polymerase chain reaction (qPCR, RT-qPCR), droplet digital PCR (ddPCR), and next-generation sequencing (NGS). The kits contain enough reagents for 96 extractions (Product code: **29506009**) or for 1000 extractions (Product code: **29514201**).

### 3.1 Basic principle

#### Illustrated procedure

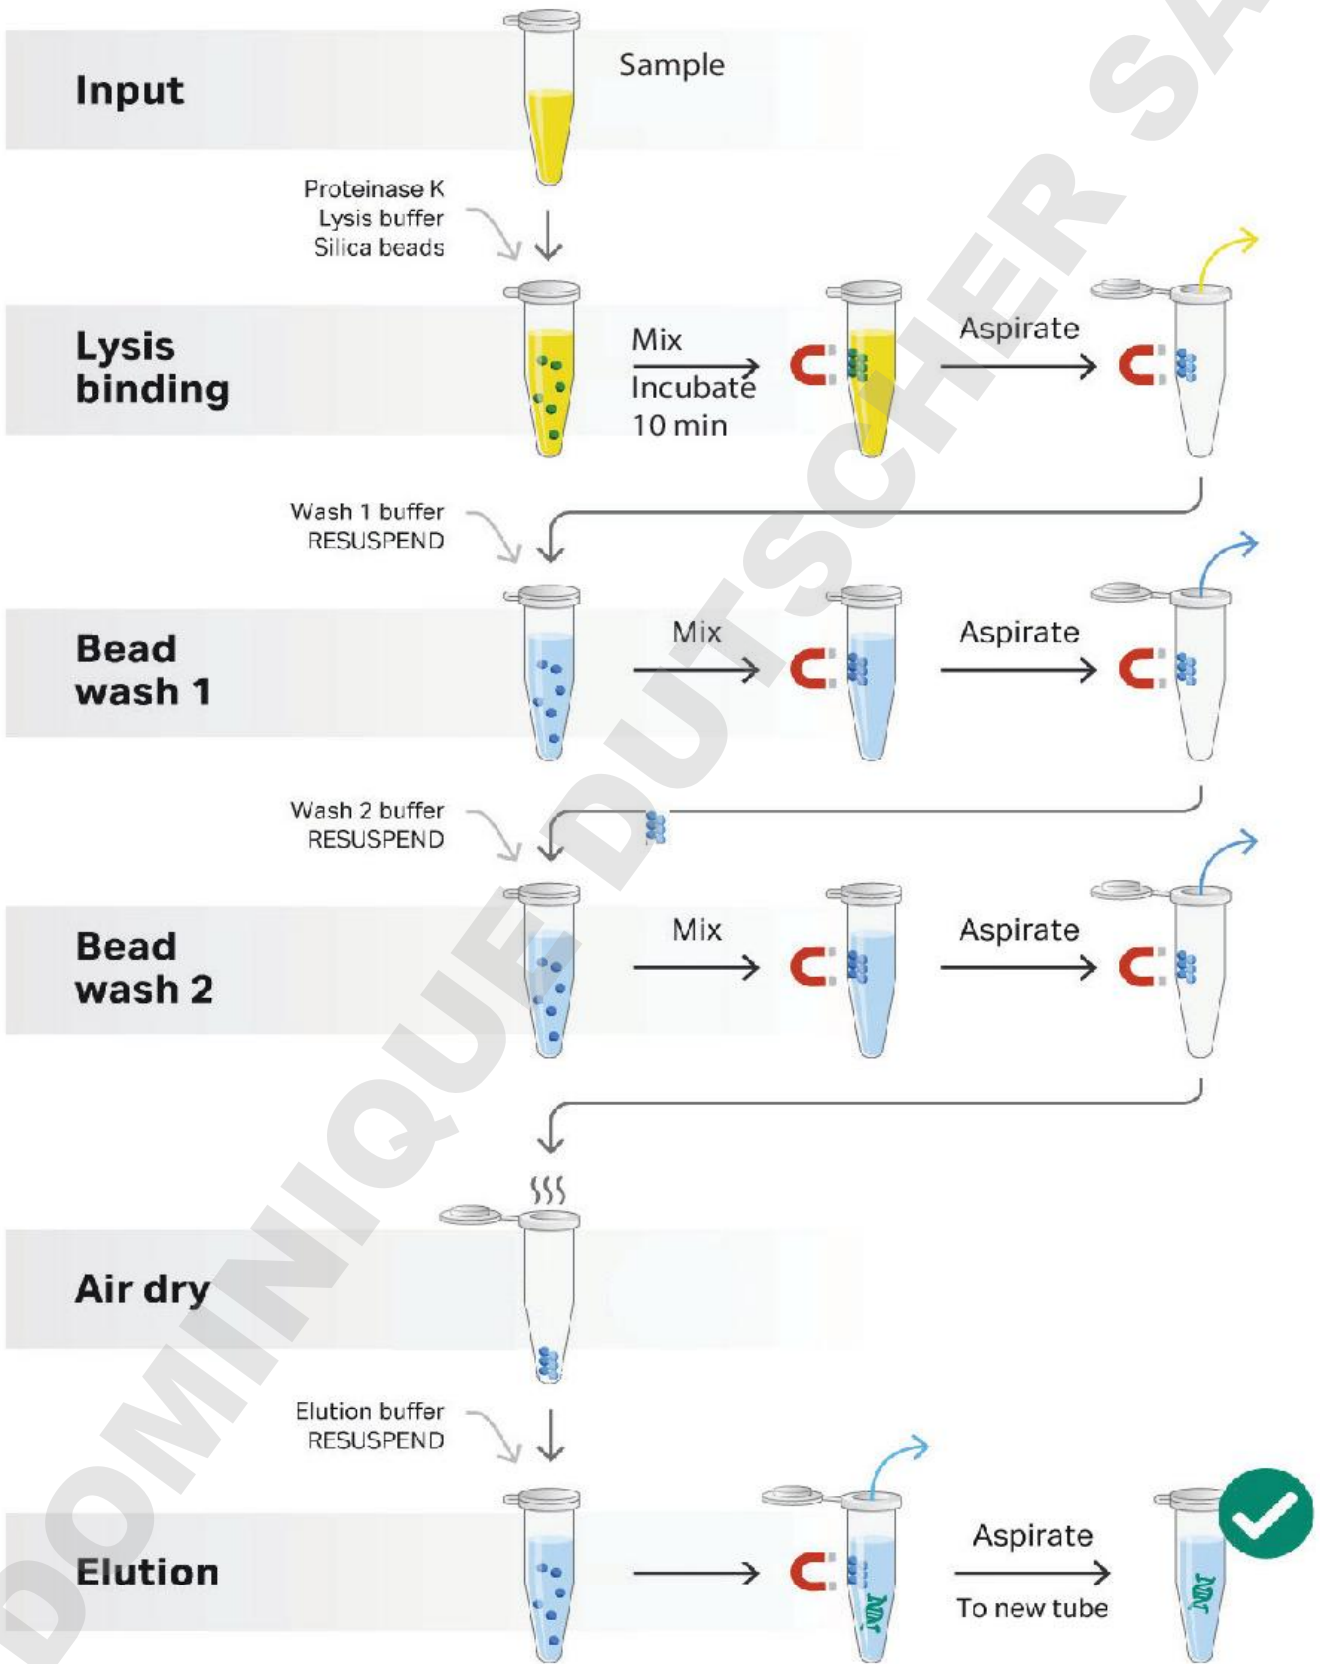


Fig 1. Sera Xtracta Virus/Pathogen kit workflow.

## Step procedure

Step	Comments	Component
<b>1</b> Sample binding/ lysis step	Cells are lysed by a chaotropic salt and detergent in the lysis buffer, in the presence of Proteinase K and nucleic acids are bound to the magnetic beads	Lysis Buffer Proteinase K SeraSil-Mag 400 beads SeraSil-Mag 700 beads
<b>2</b> Wash 1 (buffer)	Wash Buffer containing a chaotropic salt removes contaminants from bound nucleic acids	Wash Buffer
<b>3</b> Wash 2 (ethanol solution)	Further washing with ethanol to remove remaining contaminants	80% ethanol
<b>4</b> Drying	Excess ethanol is removed by air drying	–
<b>5</b> Elution	Nucleic acid is eluted in nuclease free water and aspirated away from the magnetic beads into a fresh tube	Nuclease free water

## 3.2 Product specifications

The Sera-Xtracta Virus/Pathogen Kit has been optimized for the isolation of nucleic acid from swab samples collected in universal transport media. For expected yields from different transport media please refer to appendices.

Sample type	Swab sample collected into Primestore™ MTM
Sample input volume	100–400 µL
Elution volume	50 µL <sup>1</sup>
Yield	Detection of 1 copy/µL in Real-Time RT-PCR <sup>2</sup>

<sup>1</sup> Recommended elution volume: the end user has the option to vary this according to downstream application requirements

<sup>2</sup> Based on the concentration of synthetic viral RNA in the input sample

## 4 Protocol

### 4.1 Reagent preparation before use of kit

#### Proteinase K

Reconstitute Proteinase K to 20 mg/mL with nuclease-free water (for example 1.5 mL added to 30 mg vial). Reconstituted enzyme is stable for at least 4 months when stored at 2°C to 8°C.

#### 80% ethanol wash solution (Wash 2)

Prepare an 80% ethanol wash solution. **Note:** Prepare enough 80% ethanol for 950  $\mu$ L per extraction reaction. Use 100% absolute ethanol and nuclease-free water.

#### SeraSil-Mag bead working solution

Prepare a working solution of SeraSil-Mag 400 and SeraSil-Mag 700 beads (supplied as separate vials in the kit) in a 1:1 ratio. Vortex SeraSil-Mag beads thoroughly before each is added to the pre-mixture and then again prior to use. **Note:** Prepare sufficient bead volume for 20  $\mu$ L bead mixture per reaction.

#### Elution

Pre-heat an aliquot of nuclease-free water for final nucleic acid elution from the beads, using a heated incubator set at 70°–75°C. **Note:** typical elution volume is 50  $\mu$ L per reaction.

### 4.2 Protocol for nucleic extraction from 100–400 $\mu$ L sample

#### Step 1: Lysis and Nucleic Acid Binding

1. Add 10  $\mu$ L of **Proteinase K** Solution to a 1.5–2.0 mL microcentrifuge tube.
2. Add 100–400  $\mu$ L of sample to the tube.
3. Add 20  $\mu$ L of **SeraSil-Mag bead working solution** (as prepared above) and mix the solution by slowly pipetting up/down 5–10 times **Note:** Prior to adding, ensure SeraSil-Mag bead tubes are thoroughly vortexed and mix the beads frequently during pipetting.
4. Add 570  $\mu$ L of **Binding/Lysis Reagent** to the 1.5–2.0 mL microcentrifuge tube. **Note:** Solution is highly viscous; pipette slowly to avoid a void volume in the tip and excess foaming.

5. Ensure thorough mixing of the solution, cap and place tube on vortex mixer set a medium speed for 1 min. Pulse spin contents in a microcentrifuge to bring contents down.
6. Incubate tube on heat block set to 60°C for 10 min. **Note:** Heat step enhances lysis and activates Proteinase K enzyme. If precipitation is evident, quick spin tube to bring down contents.
7. Place tube on magnet stand for 1 min or until the solution becomes clear. Without disturbing bound beads, carefully remove the entire supernatant.

## Step 2: Wash the Bound RNA/DNA

1. Remove the sample tube from the magnet stand, add 950 µL **Wash Buffer (Wash 1)** and mix the solution by slowly pipetting up/down 5–10 times.
2. Ensure thorough mixing of the solution, cap and place tube on vortex mixer set a medium speed for 1 min. Pulse spin contents in a microcentrifuge to bring contents down.
3. Place the tube on a magnet stand for 1 min or until the solution becomes clear. Without disturbing bound beads, carefully remove the entire supernatant.
4. Remove the tube from the magnet stand and add 950 µL of freshly prepared **80% ethanol (Wash 2)** to the sample tube.
5. Mix tube contents by slowly pipetting the contents up/down 5–10 times. Pulse spin contents in a microcentrifuge to bring contents down.
6. Place the tube on the magnet stand for 1 minute or until the solution becomes clear. While on the magnet stand, carefully remove the supernatant without disturbing the pellet.
7. Briefly remove the tube from the magnet stand allowing the beads to sink towards the bottom of the tube. Note: This should take 3–5 s.
8. Place the tube back onto the magnet. When the beads collect to the magnet use a 10 or 20 µL pipette to carefully remove any remaining ethanol. **Important:** It is important to ensure that all the ethanol is removed.
9. Remove the tube from the magnetic stand and allow the beads to air-dry for 2 min.



### Step 3: Elution of RNA/DNA

1. Add 50 µL of pre-heated (70°C–75°C) **nuclease-free water** to each sample tube. Pipette up and down slowly until all the beads are removed from the side of the tube and the entire bead mass is at the bottom of the tube (pulse spin the tubes in a microcentrifuge if needed)
2. Place the tube on the magnet stand for 1 min or until contents are clear.
3. With the tube on the magnet, carefully transfer the eluate, containing the extracted RNA/DNA sample to a new microcentrifuge tube.

#### Notes;

A pulse spin in a microfuge is strongly recommended before magnet settling to ensure all the liquid sample in the tube is collected together in a single bulk volume at the bottom of the tube. Isolated droplets on the tube walls or trapped under the tube lid will affect results.

### 4.3 Storage of recovered nucleic acid


The protocol recommends elution of the sample in nuclease free water. Purified DNA or RNA may be stored at 2°C–8°C for a short period when used immediately for analysis and/or downstream molecular biology/analytical applications. For long term storage aliquot and store purified DNA isolates at -20°C and RNA isolates at -80°C or less (user might consider using standard TE buffer, pH. 8–8.5 for DNA or 1 mM sodium citrate, pH 6.5 for RNA).

## 5 Appendices

For all experiments, the recovery of nucleic acid has been demonstrated using Real-Time RT-PCR assay, performed in technical duplicates using TaqPath™1-Step RT-qPCR Master Mix, CG (ThermoFisher Scientific) and CDC 2019 Novel Coronavirus (2019-nCoV) Diagnostic Panel primers (N1, N2, N3 targeting three regions of SARS-CoV-2 nucleocapsid gene and RNase P primers targeting human RNase P gene, Integrated DNA Technologies).

### 5.1 Recovery of synthetic SARS-CoV-2 RNA


Experiments were carried out to test the extraction of a synthetic SARS-CoV-2 RNA (N gene, Seracare) spiked into a diluent consisting of a suspension of human cells ( $\sim 3 \times 10^5$ /mL) in 400  $\mu$ L Primestore MTM (FDA approved transport media) to mimic a clinical sample. Averages of between 2 and 6 replicates per condition were obtained from multiple experiments, by multiple operators using two batches of the extraction kit reagents. Cytiva Sera-Xtracta Virus/Pathogen kit allows for confident detection of viral RNA down to 1 copy/ $\mu$ L in the input sample. For comparison with the CDC published data for the 2 referenced QIAGEN kits please refer to the table below (CDC Division of Viral Diseases, CDC-006-00019).

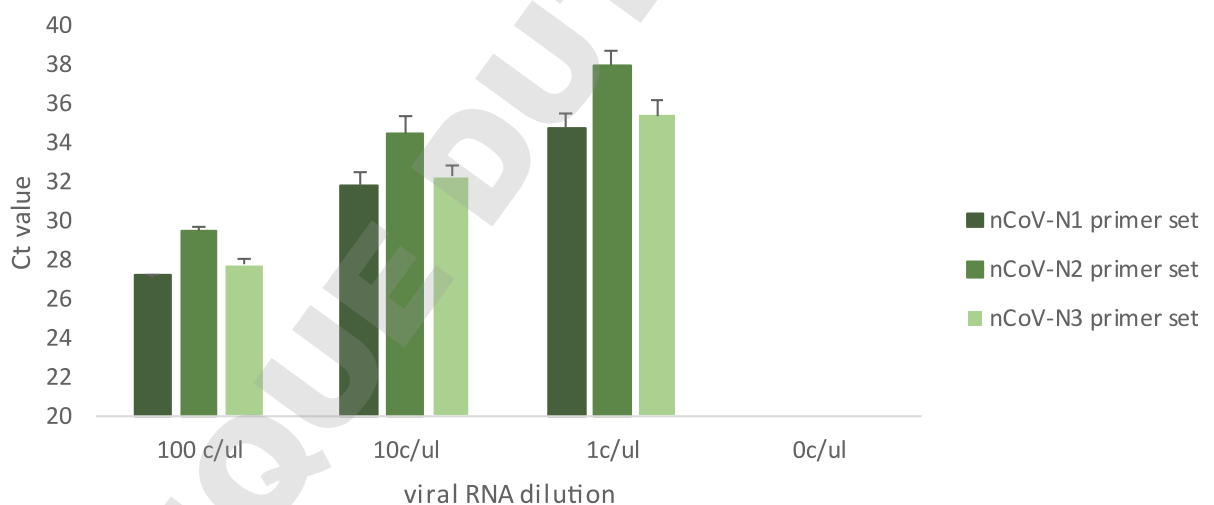

RNA Target Conc 1 copy/ $\mu$ L in MTM	nCoV-N1	nCoV-N2	nCoV-N3
Cytiva Sera-Xtracta Virus/Pathogen kit (Primestore MTM, 400 $\mu$ l)	<b>34.6</b>	<b>37.9</b>	<b>35.4</b>
QIAGEN QIAmp DSP Viral RNA Mini kit (VTM identity and volume not disclosed)	32.8	35.4	32.7
QIAGEN EZ1 DSP Virus kit (VTM identity and volume not disclosed), LOD > 3.16 copies/ $\mu$ L	35.4	–	–


## 5.2 Comparative performance of Sera-Xtracta Virus/Pathogen kit

We have compared the performance of the Sera-Xtracta Virus/Pathogen kit for the extraction of a synthetic SARS-CoV-2 RNA (N gene, Microbiologics/Virapur) spiked at between 1 and 10 000 copies/ $\mu$ L into a diluent consisting of a suspension of human cells ( $\sim 3 \times 10^5$ /mL) in 200  $\mu$ L of Primestore MTM to mimic a clinical sample with that of one of the CDC recommended extraction kits (QIAGEN QIAamp MinElute Virus Spin kit ) for COVID-19 virus detection (as per manufacturer's instructions). Data from 3 independent experiments are presented below and confirm that both kits are able to detect the presence of viral RNA down to 1 copy/ $\mu$ L in the input sample.

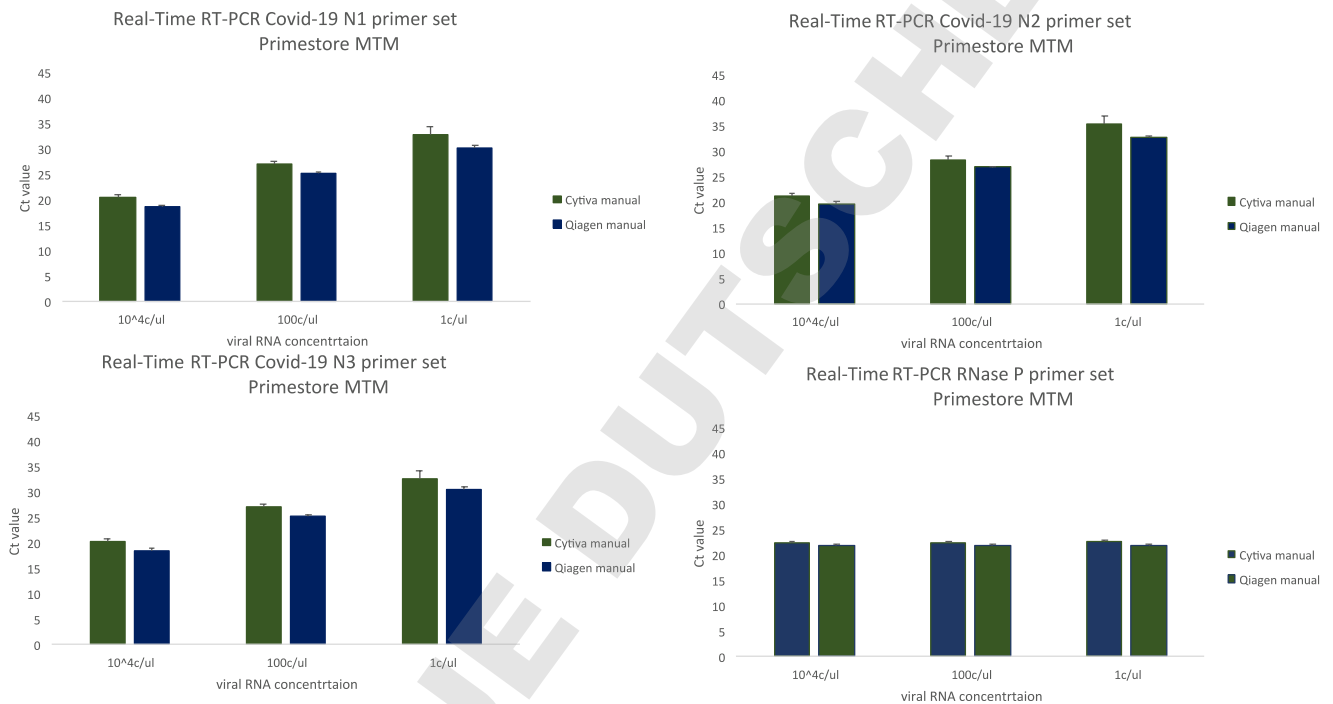


## 5.3 Use of an automated protocol

We have assessed the use of the Sera-Xtracta Virus/Pathogen kit in an automated system (Kingfisher DUO, Thermo Scientific Inc). Experiments were carried out to test the extraction of a synthetic SARS-CoV-2 RNA (N gene, AB Scientific) in 200  $\mu\text{L}$  of the Primestore MTM transport media containing between 1 and 10 000 copies/ $\mu\text{L}$  of viral RNA in the presence of human cells as described previously. Data from 2 independent experiments from both manual and automated extraction method are shown below and confirm that both methods enable detection of the viral RNA down to 1 copy/ $\mu\text{L}$  in the input sample. For further information, the automation script description is available upon request.

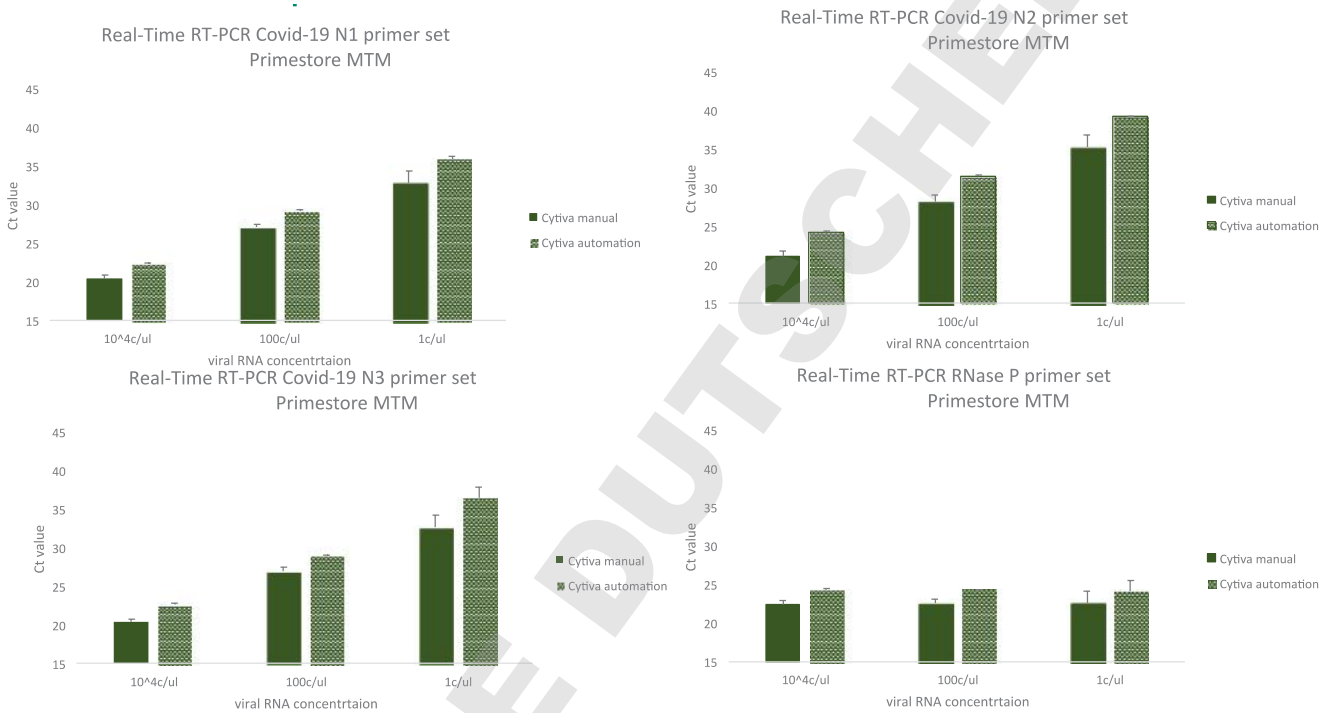

## 5.4 Use with other UTM / VTM media

Sera-Xtracta Virus/Pathogen kit has been optimized for viral nucleic acid extraction from Primestore MTM transport media. We have tested kit's performance when using alternative UTM using automated protocol on Kingfisher DUO. 200  $\mu\text{L}$  of Copan UTM (BD) and 200  $\mu\text{L}$  of Primestore MTM containing human cells ( $\sim 3 \times 10^5/\text{mL}$ ) was spiked with a synthetic SARS-CoV-2 RNA at 100 and 10 copies/ $\mu\text{L}$  and processed as described before. Extracted samples were subjected to Real-Time RT-PCR following CDC protocol as described previously. Data from 4 independent experiments are presented in the Figure 5 and confirm successful detection of the viral RNA load down to 100 copies/ $\mu\text{L}$  in the input sample when using alternative transport media. Please note that N3 primer set is no longer included in CDC diagnostic panel but remains as part of RUO.

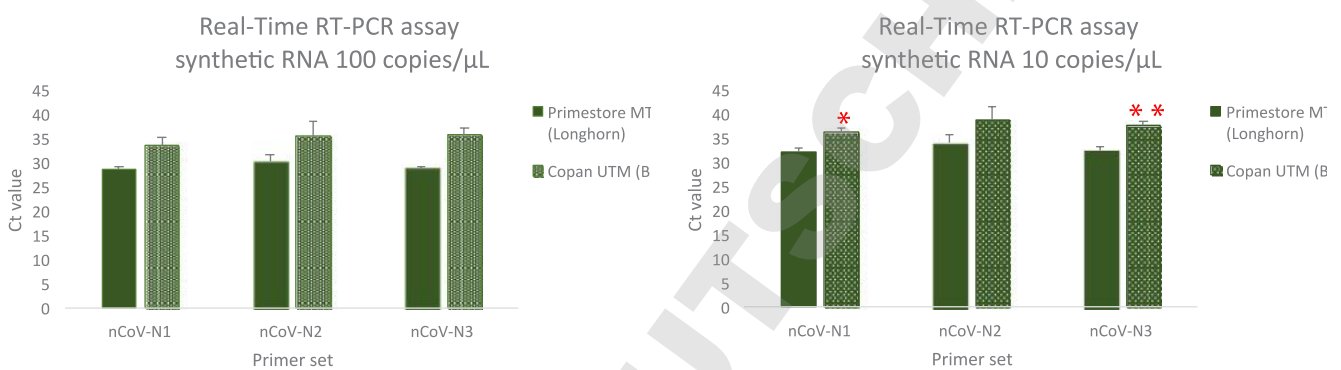


\* Undetermined in one out of 4 experiments

\*\* Undetermined in two out of 4 experiments

## 6 Performance using recombinant viral particles

Successful lysis and the release of a nucleic acid material from viral particles are critical for the efficient extraction process and reliable detection of viral pathogens. We have tested the performance of Sera-Xtracta Virus/Pathogen Kit using non-replicative recombinant Sinbis virus containing sequences from the SARS-CoV-2 (AccuPlex™ SARS-CoV-2 reference material, SeraCare). Like Coronaviruses, Sinbis viruses contain a nucleocapsid enclosed in a lipid envelope providing a highly relevant control allowing to extrapolate the efficiency of RNA extraction to samples containing SARS-CoV-2. The product is formulated in viral transport media mimicking a swab sample and contains approximately 5 viral copies/ $\mu\text{L}$ . The negative reference material included in the kit contains the sequence of human RNase P gene that serves as the assay control to eliminate the possibility of false positives. 200  $\mu\text{L}$  of SeraCare material was processed using Sera-Xtracta Virus/Pathogen kit, eluted in 50  $\mu\text{L}$  of nuclease-free water and subjected to Real-Time RT-PCR assay following CDC protocol as described before.

Data from 3 independent experiments are presented in the figure below and confirm successful extraction of RNA from viral particles allowing for confident detection of the virus present at 5 copies/ $\mu\text{L}$  in the input sample.

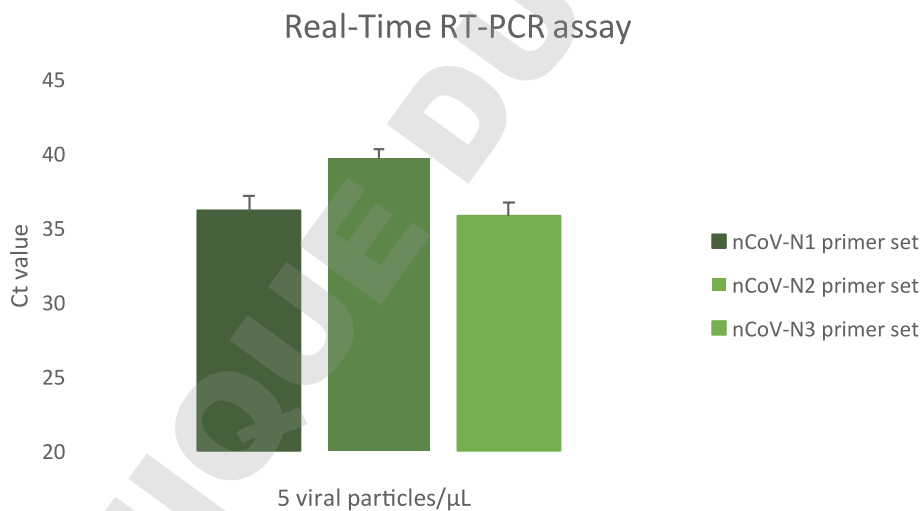

## 7 Related products

Product	Pack size	Product code
Sera Xtracta Cell-Free DNA Kit	96 purifications (2ml input)	29437807
Sera Xtracta Genomic DNA Kit	96 purifications	29429140
RNAspin Mini Kit	20 preps 50 preps 250 preps	25050070 25050071 25050072
RNAspin 96 Kit	4 x 96 preps	25050075
Sera-Mag Select	5 mL 60 mL 450 mL	29343045 29343052 29343057
PuRe Taq Ready-To-Go PCR beads	Multiwell plate, 96 reactions	27955701
	Multiwell plate, 5 x 96 reactions	27955702
	0.5 mL tubes, 100 reactions	27955801
	0.2 mL hinged tube with cap, 96 reactions	27955901
GenomiPhi V2 DNA amplification kit	100 reactions	25660031
	500 reactions	25660032
Ready-To-Go GenomiPhi V3 DNA amplification kit	10 purifications	28903466
	100 purifications	28903470
	200 purifications	28903471
GFX 96 PCR Purification Kit	96 purifications	28903445
Blood genomicPrep Mini Spin Kit	10 purifications	10 purifications
	50 purifications	50 purifications
	250 purifications	250 purifications
Tissue and Cells genomicPrep Mini Spin Kit	50 purifications	28904275
	250 purifications	28904276
MagRack Maxi	15 mL / 50 mL tubes	28986441
MagRack 6	1.5mL / 2.0 mL microtubes	28948964



cytiva.com

Cytiva and the Drop logo are trademarks of Global Life Sciences IP Holdco LLC or an affiliate.

SeraSii-Mag and Sera-Xtracta, are trademarks of Global Life Sciences Solutions USA LLC or an affiliate doing business as Cytiva.

AccuPlex is a trademark of SeraCare Life Sciences, Inc. Primestore is a trademark of Longhorn Vacines . TaqPath is a trademark of ThermoFisher Scientific

All other third party trademarks are the property of their respective owners.

© 2020 Cytiva

All goods and services are sold subject to the terms and conditions of sale of the supplying company operating within the Cytiva business. A copy of those terms and conditions is available on request. Contact your local Cytiva representative for the most current information.

For local office contact information, visit [cytiva.com/contact](https://www.cytiva.com/contact).

29513970 AC 08/2020