Biosigma SpA
a Dominique Dutscher Company
Via Valletta, 6 | 30010 Cantarana di Cona (VE), Italy | Tel. ++39 0426 302224 (r.a.) |
Fax ++39 0426 302228 E-mail info@biosigmaeu.com | http://www.biosigma.com |
www.biosigma.it

SCHEDA TECNICA PRODOTTO – TECHNICAL DATA SHEET

Low Binding PROTEIN CLEARLock® CLEARLine® Microtubes



I microtubi Low Binding sono progettati per ridurre al minimo la possibile perdita del materiale soprattutto quando si lavora con basse concentrazioni.
I microtubi Low Binding forniscono la soluzione ideale sia per la preparazione che per la conservazione a lungo termine dei campioni.
Ogni lotto è certificato privo di DNA umano, DNasi, RNasi, ATP, endotossine, e inibitori della PCR.
The Low Binding microtubes are designed to minimize sample loss especially when working with low concentrations.
The Low Binding microtubes provide the ideal solution for both sample preparation and long-term storage.
Each batch is certified free from human DNA, DNase, RNase, ATP, endotoxins, and PCR inhibitors.

Caratteristiche Principali:

- Elevato recupero delle Proteine
- Il tappo di sicurezza impedisce qualsiasi apertura involontaria durante l'uso
- La chiusura ermetica evita l'evaporazione durante la conservazione a lungo termine
- Tappo scrivibile e perforabile
- Graduati con area di scrittura
- Trasparenza eccellente
- Centrifugazione massima 30.000g
- Intervallo di temperatura da -80°C a + 100°C
- Autoclavabili a +121°C per 20 minuti
- Liberi da Metalli
- Confezionati in buste con sistema di apertura e chiusura
- Particolarmente adatti per tutte le applicazioni in Biochimica
- In Polipropilene medicale, Non Citotossico – Non Emolitico, indicato per la conservazione dei campioni chimici e biologi
- Lotti certificati* privi di DNA umano, DNasi, RNasi, endotossine, ATP, e inibitori della PCR
  Certificato di analisi scaricabile dal nostro sito web www.biosigma.it
- Smaltimento del prodotto: i prodotti NON utilizzati sono considerati non pericolosi e possono essere riciclati previo opportuni trattamenti.

Main features:

- *High Protein recovery*
- *The safety cap prevents any accidental opening during use*
- *Hermetic closure prevents evaporation during long-term storage*
- *Writable and pierceable cap*
- *Graduates with writing area*
- *Excellent transparency*
- *Maximum centrifugation 30.000g*
- *Temperature range from -80°C to +100°C*
- *Autoclavable at +121°C for 20 minutes*
- *Metals Free*
- *Packaged in bags with an opening and closing system*
- *Especially suited for all the Biochemistry applications*
- *In Polypropylene medical grade, Non Cytotoxic - Non Hemolytic, suitable for the conservation of chemical and biological samples*
- *Certified batches* free from human DNA, DNase, RNase, endotoxins, ATP, and PCR inhibitors*
  Certificate of analysis downloadable from our website www.biosigma.com
- *Product disposal: the products NOT used are considered non-hazardous and can be recycled after appropriate treatment. Used devices are to be*

SCHEDA TECNICA PRODOTTO – TECHNICAL DATA SHEET

I dispositivi usati sono da considerarsi potenzialmente infetti (rifiuti pericolosi) e smaltiti secondo le vigenti normative.

■ Smaltimento dell'imballaggio: raccogliere il materiale di imballaggio e gettarlo negli appositi contenitori di raccolta presso la propria organizzazione


considered potentially infectious (hazardous waste) and disposed of according to current regulations.

■ *Packaging disposal: collect the packing material and place it in the appropriate collection containers at your organization.*

Microtubi, Low Binding PROTEIN

Informazioni per l'ordine/*Ordering information*:


Codice - *Part no*	**Descrizione-*Description***	**Conf. interna** ***Inner pack***	**Conf. est.** ***Box***
CL05.0100PLB	Protein Low Binding CLEARLock® CLEARLine® Microtubes 0.5 ml	bag/100	500
CL15.0050PLB	Protein Low Binding CLEARLock® CLEARLine® Microtubes 1.5 ml	bag/50	200
CL20.0050PLB	Protein Low Binding CLEARLock® CLEARLine® Microtubes 2 ml	bag/50	200

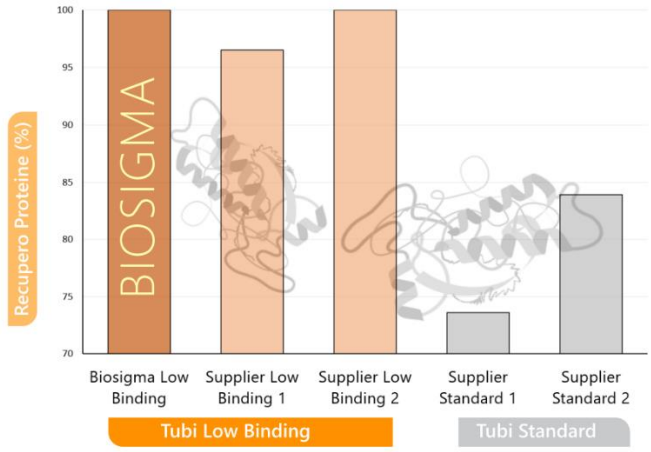

RECUPERO DELLE PROTEINE CON LE MICROPROVETTE BIOSIGMA LOW BINDING CLEARLOCK ® CLEARLINE ® A CONFRONTO CON ALTRI PRODUTTORI LOW BINDING E STANDARD

PROTEIN RECOVERY WITH CLEARLOCK® CLEARLINE® LOW BINDING MICROTUBES COMPARED WITH OTHER LOW BINDING AND STANDARD MICROTUBE SUPPLIERS

Dimensioni / *Dimensions*

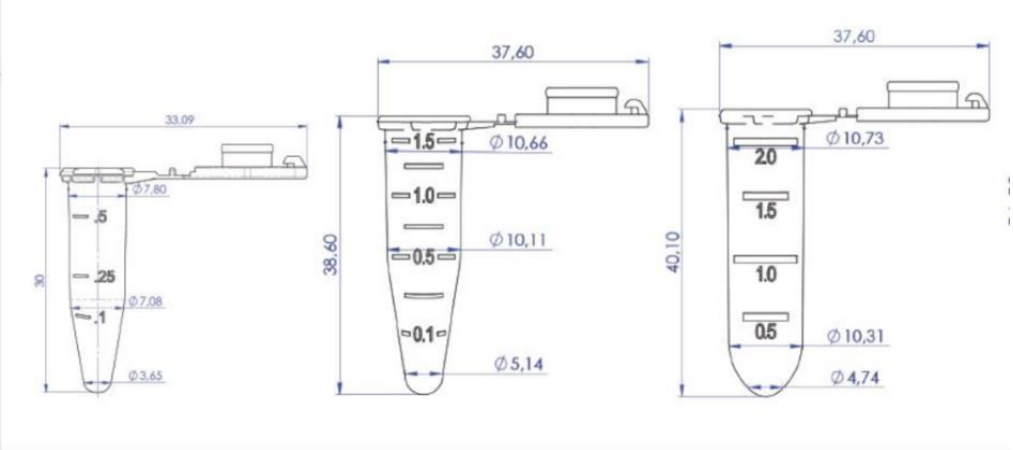

FABBRICANTE: *BIOSIGMA SpA Via Valletta, 6 30010 - Cantarana di Cona (VE) - ITALY*
MANUFACTURER: *Tel. +39.0426.302224 - Fax +39.0426.302228 E-mail: info@biosigma.com*
http://www. biosigma.com