# eppendorf



# Move It!

Multiple sample transfer between different formats now becomes fast and secure NEW: Eppendorf Research® plus and Eppendorf Xplorer® plus Move It® adjustable spacing pipettes

# Double Your Performance

#### Maximizing efficiency

Do you frequently switch between different consumable formats i.e. tubes to plates? With the new Move It pipettes you can easily switch between various formats; reducing your throughput time by 50% while increasing reproducibility.

#### Safe sample transfer

For a safe sample transfer, the spacing adjustment is vibration-free, easy, and fast. By just a simple turn of the adjustment knob, the tip distance is modified.

# 1. Maximizing Efficiency


#### Easy and fast format change

Often, single channel pipettes are used for multiple sample transfer from one vessel type to another. This can be time-consuming and inconvenient, especially when throughput increases.

Multiple sample transfers between different vessel types and formats become possible with the new Move It pipettes. Instead of pipetting many times, four to twelve samples can now be moved simultaneously. This not only saves you valuable time, it further increases the reproducibility of your results.


#### **Defined settings for quick switches**

Switching between source and destination vessels made simple by using the spacing control. These pipettes can easily be adjusted manually with pre-defined settings for different plate formats. All you have to do is to set the spacing control to 384, 96, 48, 24 or 12-well plates using the indicated scale. This enables quick switches back and forth, between two formats, by manually operating the adjustment knob.

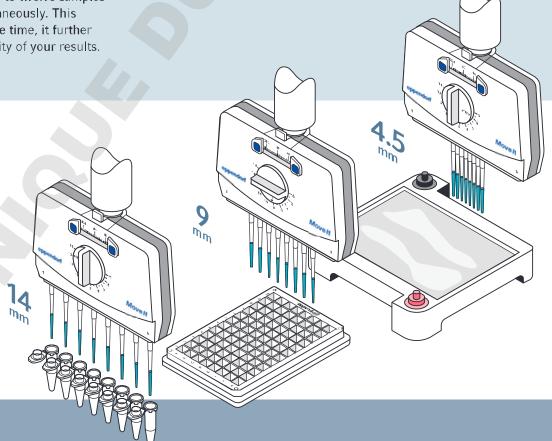

#### **Example applications**

- > Blood analysis
- > FACS analysis
- > Cell Based Assays
- > Cell Culture
- > ELISA
- > PCR
- > Mouse genotyping

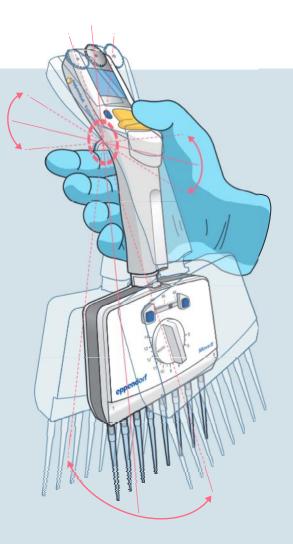


#### Optimal balance for a relaxed hand


Need a break? With a natural and relaxed hand position the demand for a break decreases. Move It pipettes reduce hand fatigue to a minimum. This is achieved by an optimized balance of the pipette. The user also benefits from convenient visibility of tips and samples. Enjoy a stress-free operation the whole day long.

PhysioCare Concept

#### Rotatable pipette head - 360°

All Move It pipettes are designed without the need of tubing. Thus, the pipette head is completely rotatable. The user benefits from comfortable readability of the display. This not only supports an ergonomic and relaxed body posture, it also ensures fast identification of all parameters; saving you valuable time.

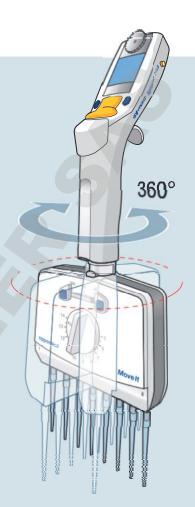

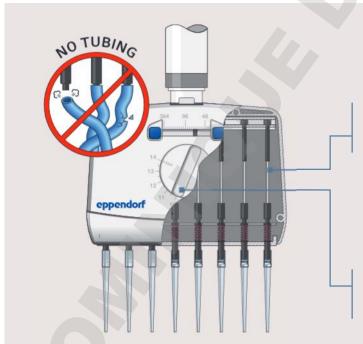

# 2. Safe Sample Transfer

#### Tubeless system for reliability and reproducible results

The piston cylinder system is directly connected to the nose cone.

The user therefore benefits from special advantages:

- > Lack of heat transfer to air-cushion from motor or hand for stable temperature for higher precision and reproducibility
- > Easy autoclavability\* for reduced contamination risk
- > Lack of possible cable tangle and tubing-porosity for consistently reliable robustness and precision
- > Less maintenance requirements compared to pipettes with tubing system

#### Adjustment knob for smooth liquid transfer

Since no motor is used, format changes don't cause vibrations; enabling liquid transfers without the risk of dripping.

\* Xplorer plus lower partionly, and Research plus fully autoclavable



# Move It Keeps The Balance For You

#### **Business Manager Peter Schmidt**

When developing the adjustable spacing pipettes, our goal was to keep the ideal balance in the hand. As the lower part of the pipette gained weight, we faced a challenge. An external study revealed that a good balance is more important for the user than the total weight. Encouraged by this, we replaced some inner parts of the pipette with metal parts. The result is a well-balanced pipette supporting ergonomic working conditions.



#### Move It - You have the choice


Mechanical Research plus pipettes are the workhorses for each lab. The Xplorer electronic pipettes with highest variety of functions are the ideal instrument if you need intuitively and precisely adjustable parameters. reproducible and accurate results while experiencing fatigue-free pipetting.



> Tip spacing adjustable manually > Intuitive, direct, and vibration-free > Liquid transfers without dripping

#### **Tubeless system**

> Stable temperature in air-cushion > Consistently reliable robustness and precision > Easy autoclavability\* > Reduced maintenance requirements



#### Rotatable pipette head - 360°


- > Comfortable readability of display
- > Ergonomic and relaxed body posture
- > Fast identification of parameters

#### Spacing control

- > For adjusting source and destination formats
- > Easy assignment to 384-. 96-, 48-, 24-, and 12-well plates
- > Quick switches backwards and forwards between the formats

#### Adjustable tip spacing

- > For microplates, sample tubes, tubes in holders, and agarose gels
- > Tip spacing freely selectable between 4.5 and 33 mm





All models available as electronical Xplorer plus and mechanical Research plus.



	Type of tips	epT.I.P.S.®			epT.I.P.S.® 384		
Vessel Format	Pipette Electronical Mechanical	Eppendorf Xplorer® plus, Eppendorf Research® plus			Eppendorf Xplorer® plus, Eppendorf Research		
	No. of channels	4	6	8	8	12	
	Volume (μL)	300 / 1,200	300 / 1,200	300 / 1,200	20 / 100	20 / 100	
	Tip distance (mm)	9–33	9–20	9–14	4.5–14	4.5-9	
	384 Wells (Tip distance 4.5 mm)	-	-		-	•	
	96 Wells (Tip distance 9 mm)			•	•	•	
	48 Wells (Tip distance 13 mm)	•			•	-	
	24 Wells (Tip distance 19 mm)		•	-	-	-	
	12 Wells (Tip distance 26 mm)		-	-	-	-	
	1.5 mL / 2.0 mL Tube (Tip distance 14, 18, 20 mm)	14, I8, 20 rm	4, 18, 20 mm	14 mm	14 m~	-	
( <u>)</u>	Agarose gel	÷	·	Ė	•	•	

<sup>\*</sup> I imited suitability due to volume and size of tips



> Speed up your laboratory work and go to: https://handling-solutions.eppendorf.com/liquid-handling/pipetting-facts/time-saving/



# Eppendorf Research® plus Move It\* (mechanical, multichannel, variable volume)

# Eppendorf Xplorer® plus Movelt® (electronical, multichannel, variable volume, incl. c

No. of channels	Volume	Color code	Order no.
4-channel	<b>15–</b> 300 μL	orange	3125 00 <b>0 150</b>
	<b>50–1,</b> 200 μL	dark green	3125 00 <b>0 18</b> 4
6-channel	15–300 μL	orange	3125 000 168
	<b>50–1,</b> 200 μL	dark green	3125 00 <b>0 1</b> 92
8-channel	1-20 μL	light pink	<b>3</b> 125 00 <b>0 117</b>
	5–100 μL	light yellow	3125 000 133
	<b>15–</b> 300 μL	orange	3125 00 <b>0 17</b> 6
	<b>50–</b> 1,200 μL	dark green	<b>3</b> 125 00 <b>0</b> 20 <b>6</b>
12-channel	1-20 μL	light pink	3125 000 125
	5-100 μL	light yellow	3125 00 <b>0 141</b>

(electronical, multichannel, variable volume, incl. charger)					
No. of channels	Volume	Color code	Order no.		
4-channel	<b>15–</b> 300 μL	orange	4861 000 816		
	<b>50–1,</b> 200 μL	green	4861 000 833		
6-channel	<b>15–</b> 300 μL	orange	4861 000 817		
	<b>50–1,</b> 200 μL	green	4861 000 834		
8-channel	1-20 μL	light pink	<b>486</b> 1 00 <b>0</b> 7 <b>81</b>		
	5–100 μL	light yellow	<b>4</b> 8 <b>6</b> 1 00 <b>0</b> 79 <b>4</b>		
	<b>15–</b> 300 μL	orange	4861 000 818		
	<b>50–1,200</b> μL	green	4861 000 835		
12-channel	1-20 μL	light pink	4861 000 782		
	5–100 μL	light yellow	4861 000 795		

#### ep Dualfilter T.I.P.S.® 384

Purity grade	Type of packaging	Tip size	Color code	Smallest tip distance	Order no.
Rack	ep Dualfilter 1.1.P.S.® 384,	0.1-20 μL	light pink	4.5 mm	0030 078 403
(PCR clean, sterile)	$3,840 \text{ tips} (10 \text{ racks} \times 384 \text{ tips})$	0.5–100 μL	light yellow	4.5 mm	0030 078 411

#### ep Dualfilter T.I.P.S.®

Purity grade	Type of packaging	Tip size	Color code	Smallest tip distance	Order no.
Rack (PCR clean, sterile)	ep Dualfilter T.I.P.S. <sup>3</sup> , 960 tips (10 racks x 96 tips)	20-300 μL	orange	9 mm	0030 077 563
	ep Du <b>al</b> filter T.I.P.S. <sup>3</sup> , 480 tips (5 racks × 96 tips)	<b>50-</b> 1,250 μL L	■ dark green	9 mm	0030 077 <b>7</b> 50

> Find the entire product range of tips at www.eppendorf.com/tips



> For more information on pipette service go to www.eppendorf.com/epServices

Your local distributor: www.eppendorf.com/contact

Eppendorf  $AG \cdot Barkhausenweg \ 1 \cdot 22339 \ Hamburg \cdot Germany eppendorf@eppendorf.com \cdot www.eppendorf.com$ 

www.eppendorf.com

Eppendorf®, the Eppendorf Brand Design, Eppendorf Research®, Eppendorf Xplarer®, PhysioCare Concept®, the epServices® logo, ep Destititen T.I.R.S.®, epT.I.R.S., and Move I.® are registened tracemarks of Eppendorf AG, Germany, Eppendorf Quality™ is a tracemark of Eppendorf AG, Germany, U. S. Design Patents are listed on www.eppendorf.com/p.
All rights reselved. Including graphics are images. - Copyright © 2019 by Eppendorf AG, Carbon neutrally printed in Germany.
Order Not. AAOT 000 320/ENT/4.2T 0819/SQ/STEE