

certificate of quality

The characteristic data of the procedure of the following test kit were determined during the production control process. For more details on how the data are determined please consult the respective reference in the literature.

Spectroquant® Phosphate Cell Test, Cat. No. 1.14543

Measuring Range	0.05 - 5.00 mg/l PO ₄ -P
Photometer	Reference
Cell	16-mm* round cell
Wavelength	690 nm

* outer diameter

Specified data for procedure

Lot-specific data

Slope	see lot-specific Certificate of Analysis (CoA)
Ordinate segment	
Reagent Blank	

Data for procedure according to ISO 8466-1^[1] and DIN 38402 A51^[2]

Residual Standard Deviation	0.0137 A
Sensitivity 0.010 A (absorbance)	0.02 mg/l PO ₄ -P
Confidence Interval (P=95%)	± 0.05 mg/l PO ₄ -P
Number of Lots	64
Standard Deviation of the Method	0.022 mg/l PO ₄ -P
Variation Coefficient of the Method	0.91%

Limit of Detection/Quantification

according to APHA 1030 C^[3]

Lower Level of Detection (LLD)	0.009 mg/l PO ₄ -P
Method Detection Level (MDL)	0.019 mg/l PO ₄ -P

according to ISO TS 13530^[4] - based on standard deviation of blank samples

Limit of Detection (LOD)	0.008 mg/l PO ₄ -P
Limit of Quantification (LOQ)	0.023 mg/l PO ₄ -P

according to DIN 32645^[5] - based on standard deviation of blank samples

Detection Limit	0.005 mg/l PO ₄ -P
Determination Limit	0.018 mg/l PO ₄ -P


Accuracy/Trueness/Precision according to DIN ISO 5725-1^[6] (in the middle of the measuring range)

Accuracy	± 0.046 mg/l PO ₄ -P
Trueness	± 0.030 mg/l PO ₄ -P
Precision	± 0.016 mg/l PO ₄ -P

Measurement Uncertainty according to DIN ISO 11352 2013-03 (Bias according to chapter 8.3.2) ^[7] (in the middle of the measuring range)

Expanded Measurement Uncertainty (k = 2)	± 0.08 mg/l PO ₄ -P
--	--------------------------------

Relative Analytical Precision

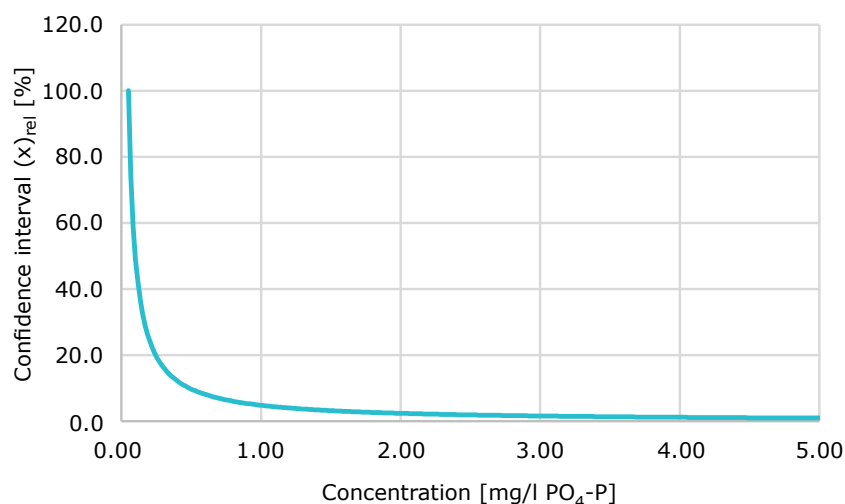

Literature

- [¹] ISO 8466-1:2021(E), Water quality – Calibration and evaluation of analytical methods, Part 1: Linear Calibration function”
- [²] DIN 38402-51:2017: German standard methods for the examination of water, waste water and sludge - general information (group A) - Part 51: Calibration of analytical methods - linear calibration (A51)
- [³] American Public Health Association, American Water Works Association, Water Environment Federation. Lipps WC, Braun-Howland EB, Baxter TE, eds. Standard Methods for the Examination of Water and Wastewater - DATA QUALITY - Method Detection Level. 24th ed. Washington DC: APHA Press; 2023.
- [⁴] ISO/TS 13530:2009: Water quality — Guidance on analytical quality control for chemical and physicochemical water analysis
- [⁵] DIN ISO 5725-1:1997-11: Accuracy (trueness and precision) of measurement methods and results - Part 1: General principles and definitions
- [⁶] DIN 32645:2008: German standard methods for the examination of water, waste water and sludge - general information (group A) - Part 51: Calibration of analytical methods - linear calibration (A51)
- [⁷] DIN ISO 11352:2013-03, Water quality – Estimation of measurement uncertainty based on validation and quality control data

Merck KGaA, Darmstadt, Germany 20.06.2024

This document is computer-generated and is valid without signature.

The life science business of Merck operates as MilliporeSigma in the U.S. and Canada.

© 2024 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved. Merck, Supelco, Sigma-Aldrich, and Spectroquant are trademarks of Merck KGaA, Darmstadt, Germany. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly available resources.

Merck Life Science KGaA, 64271 Darmstadt, Germany,
Tel. +49(0)6151 72-2440

www.sigmaaldrich.com

MERCK

Qualitätszertifikat

Die Verfahrenskenndaten für den unten genannten Testsatz wurden bei der Produktionsendkontrolle ermittelt. Nähere Einzelheiten zur Datenermittlung entnehmen Sie bitte der entsprechenden Literaturstelle.

Spectroquant® Phosphat-Küvettest, Art. 1.14543

Messbereich	0,05 - 5,00 mg/l PO ₄ -P
Photometer	Referenz
Küvette	16-mm*-Rundküvette
Wellenlänge	690 nm

* Außendurchmesser

Verfahrenskenndaten

Chargenspezifische Daten

Steigung	siehe chargenspezifisches Analysenzertifikat (CoA)
Ordinatenabschnitt	
Reagenzienblindwert	

Verfahrenskenndaten entsprechend ISO 8466-1^[1] und DIN 38402 A51^[2]

Reststandardabweichung	0,0137 E
Empfindlichkeit: 0,010 E (Extinktion)	0,02 mg/l PO ₄ -P
Vertrauensbereich (95 % Wahrscheinlichkeit)	± 0,05 mg/l PO ₄ -P
Anzahl Produktionschargen	64
Verfahrensstandardabweichung	0,022 mg/l PO ₄ -P
Verfahrensvariationskoeffizient	0,91 %

Nachweis-/Quantifizierungsgrenze

entsprechend APHA 1030 C^[3]

Nachweisgrenze (LLD)	0,009 mg/l PO ₄ -P
Nachweisgrenze des Verfahrens (MDL)	0,019 mg/l PO ₄ -P

entsprechend ISO TS 13530^[4] - basierend auf der Standardabweichung von Blindwerten

Nachweisgrenze (LOD)	0,008 mg/l PO ₄ -P
Bestimmungsgrenze (LOQ)	0,023 mg/l PO ₄ -P

entsprechend DIN 32645^[5] - basierend auf der Standardabweichung von Blindwerten

Nachweisgrenze	0,005 mg/l PO ₄ -P
Bestimmungsgrenze	0,018 mg/l PO ₄ -P


Genauigkeit/Richtigkeit/Präzision entsprechend DIN ISO 5725-1^[6] (bezogen auf die Mitte des Messbereichs)

Genauigkeit	± 0,046 mg/l PO ₄ -P
Richtigkeit	± 0,030 mg/l PO ₄ -P
Präzision	± 0,016 mg/l PO ₄ -P

Messunsicherheit entsprechend DIN ISO 11352 2013-03 (Bias entsprechend Kapitel 8.3.2)^[7] (bezogen auf die Mitte des Messbereichs)

Erweiterte Messunsicherheit (k = 2)	± 0,08 mg/l PO ₄ -P
-------------------------------------	--------------------------------

Relative analytische Präzision

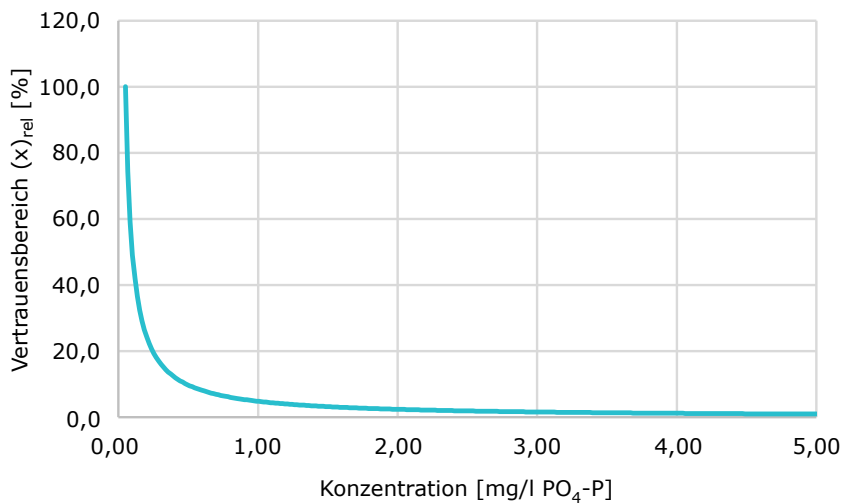

Literaturangabe

- [1] ISO 8466-1:2021(E), Water quality – Calibration and evaluation of analytical methods, Part 1: Linear Calibration function”
- [2] DIN 38402-51:2017: German standard methods for the examination of water, waste water and sludge - general information (group A) - Part 51: Calibration of analytical methods - linear calibration (A51)
- [3] American Public Health Association, American Water Works Association, Water Environment Federation. Lipps WC, Braun-Howland EB, Baxter TE, eds. Standard Methods for the Examination of Water and Wastewater - DATA QUALITY - Method Detection Level. 24th ed. Washington DC: APHA Press; 2023.
- [4] ISO/TS 13530:2009: Water quality — Guidance on analytical quality control for chemical and physicochemical water analysis
- [5] DIN ISO 5725-1:1997-11: Accuracy (trueness and precision) of measurement methods and results - Part 1: General principles and definitions
- [6] DIN 32645:2008: German standard methods for the examination of water, waste water and sludge - general information (group A) - Part 51: Calibration of analytical methods - linear calibration (A51)
- [7] DIN ISO 11352:2013-03, Water quality – Estimation of measurement uncertainty based on validation and quality control data

Merck KGaA, Darmstadt, Germany 20.06.2024

Dieses Dokument wurde maschinell erstellt und ist ohne Unterschrift gültig.

Der Unternehmensbereich Life Science von Merck tritt in den USA und in Kanada als MilliporeSigma auf.

© 2024 Merck KGaA, Darmstadt, Deutschland und/oder Tochterunternehmen. Alle Rechte vorbehalten. Merck, Supelco, Sigma-Aldrich und Spectroquant sind Marken der Merck KGaA, Darmstadt, Deutschland. Alle anderen Marken sind Eigentum der jeweiligen Inhaber. Ausführliche Informationen zu Markennamen sind über öffentlich zugängliche Informationsquellen erhältlich.

Merck Life Science KGaA, 64271 Darmstadt, Germany,
Tel. +49(0)6151 72-2440

www.sigmaaldrich.com

MERCK

certificado de calidad

Los datos característicos del procedimiento para el equipo de ensayo abajo citado se determinaron durante el control final de producción.

Para obtener más detalles sobre cómo se determinan los datos, consulte la referencia correspondiente en la bibliografía.

Spectroquant® Test en cubetas Fosfatos, art. 1.14543

Intervalo de medida	0,05 - 5,00 mg/l de PO ₄ -P
Fotómetro	Referencia
Cubeta	16-mm* cubeta redonda
Longitud de onda	525 nm

* diámetro exterior

Datos especificados para el procedimiento

Datos especificados del lote

Pendiente	consulte el Certificado de Análisis (CoA) específico del lote
Intersecto en ordenadas	
Blanco de reactivo	

Datos para el procedimiento según ISO 8466-1^[1] y DIN 38402 A51^[2]

Desviación estándar residual	0,0137 A
Sensibilidad: 0,010 A (absorbancia)	0,02 mg/l de PO ₄ -P
Intervalo de confianza (95 % de probabilidad)	± 0,05 mg/l de PO ₄ -P
Número de lotes de producción	64
Desviación estándar del procedimiento	0,022 mg/l de PO ₄ -P
Coefficiente de variación del procedimiento	0,91 %

Límite de detección/cuantificación

según APHA 1030 C^[3]

Límite inferior de detección (LLD)	0,009 mg/l de PO ₄ -P
Límite de detección del procedimiento (MDL)	0,019 mg/l de PO ₄ -P

según ISO TS 13530^[4] - basado en la desviación estándar de muestras en blanco

Límite de detección (LOD)	0,008 mg/l de PO ₄ -P
Límite de cuantificación (LOQ)	0,023 mg/l de PO ₄ -P

según DIN 32645^[5] - basado en la desviación estándar de muestras en blanco

Límite de detección	0,005 mg/l de PO ₄ -P
Límite de determinación	0,018 mg/l de PO ₄ -P


Exactitud/Veracidad/Precisión según DIN ISO 5725-1^[6] (en el medio del intervalo de medida)

Exactitud	± 0,046 mg/l de PO ₄ -P
Veracidad	± 0,030 mg/l de PO ₄ -P
Precisión	± 0,016 mg/l de PO ₄ -P

Incertidumbre de medición según DIN ISO 11352 2013-03 (Sesgo según capítulo 8.3.2)^[7] (en el medio del intervalo de medida)

Incertidumbre de medida ampliada ($k = 2$)	± 0,08 mg/l de PO ₄ -P
--	-----------------------------------

Precisión analítica relativa

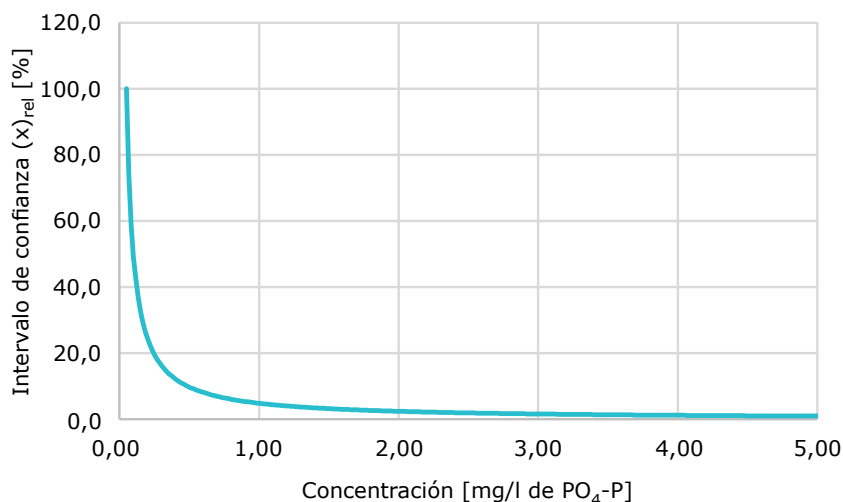

Bibliografía

- [1] ISO 8466-1:2021(E), Water quality – Calibration and evaluation of analytical methods, Part 1: Linear Calibration function”
- [2] DIN 38402-51:2017: German standard methods for the examination of water, waste water and sludge - general information (group A) - Part 51: Calibration of analytical methods - linear calibration (A51)
- [3] American Public Health Association, American Water Works Association, Water Environment Federation. Lipps WC, Braun-Howland EB, Baxter TE, eds. Standard Methods for the Examination of Water and Wastewater - DATA QUALITY - Method Detection Level. 24th ed. Washington DC: APHA Press; 2023.
- [4] ISO/TS 13530:2009: Water quality — Guidance on analytical quality control for chemical and physicochemical water analysis
- [5] DIN ISO 5725-1:1997-11: Accuracy (trueness and precision) of measurement methods and results - Part 1: General principles and definitions
- [6] DIN 32645:2008: German standard methods for the examination of water, waste water and sludge - general information (group A) - Part 51: Calibration of analytical methods - linear calibration (A51)
- [7] DIN ISO 11352:2013-03, Water quality – Estimation of measurement uncertainty based on validation and quality control data

Merck KGaA, Darmstadt, Germany 20.06.2024

Este documento se ha creado de forma automática y es válido sin firma.

La división Life Science de Merck opera como MilliporeSigma en los Estados Unidos y en Canadá.

© 2024 Merck KGaA, Darmstadt, Alemania y/o sus filiales. Todos los derechos reservados. Merck, Supelco y Sigma-Aldrich y Spectroquant son marcas comerciales de Merck KGaA, Darmstadt, Alemania. Todas las demás marcas comerciales son propiedad de sus respectivos propietarios. Tiene a su disposición información detallada sobre las marcas comerciales a través de recursos accesibles al público.

Merck Life Science KGaA, 64271 Darmstadt, Germany,
Tel. +49(0)6151 72-2440

www.sigmaaldrich.com

MERCK